
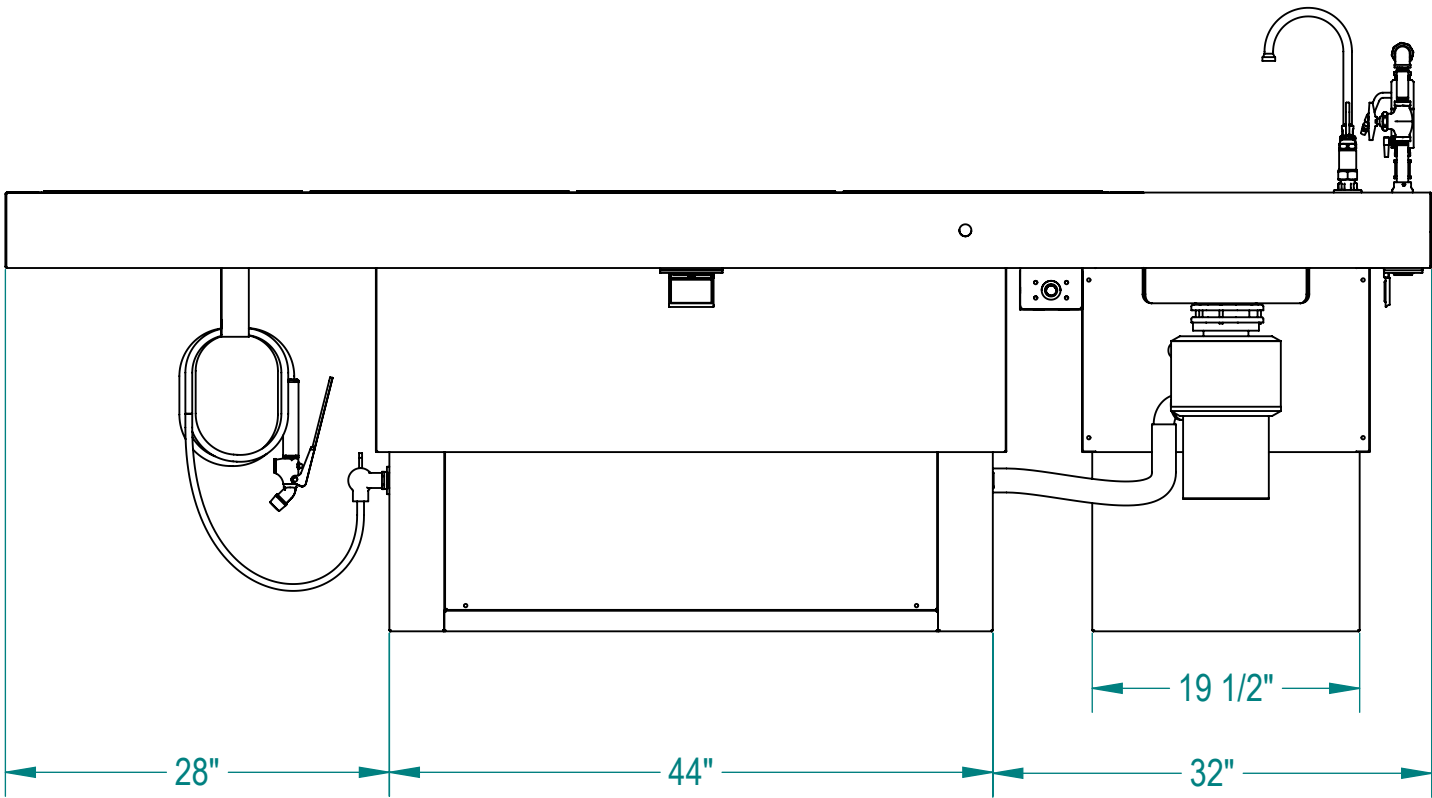
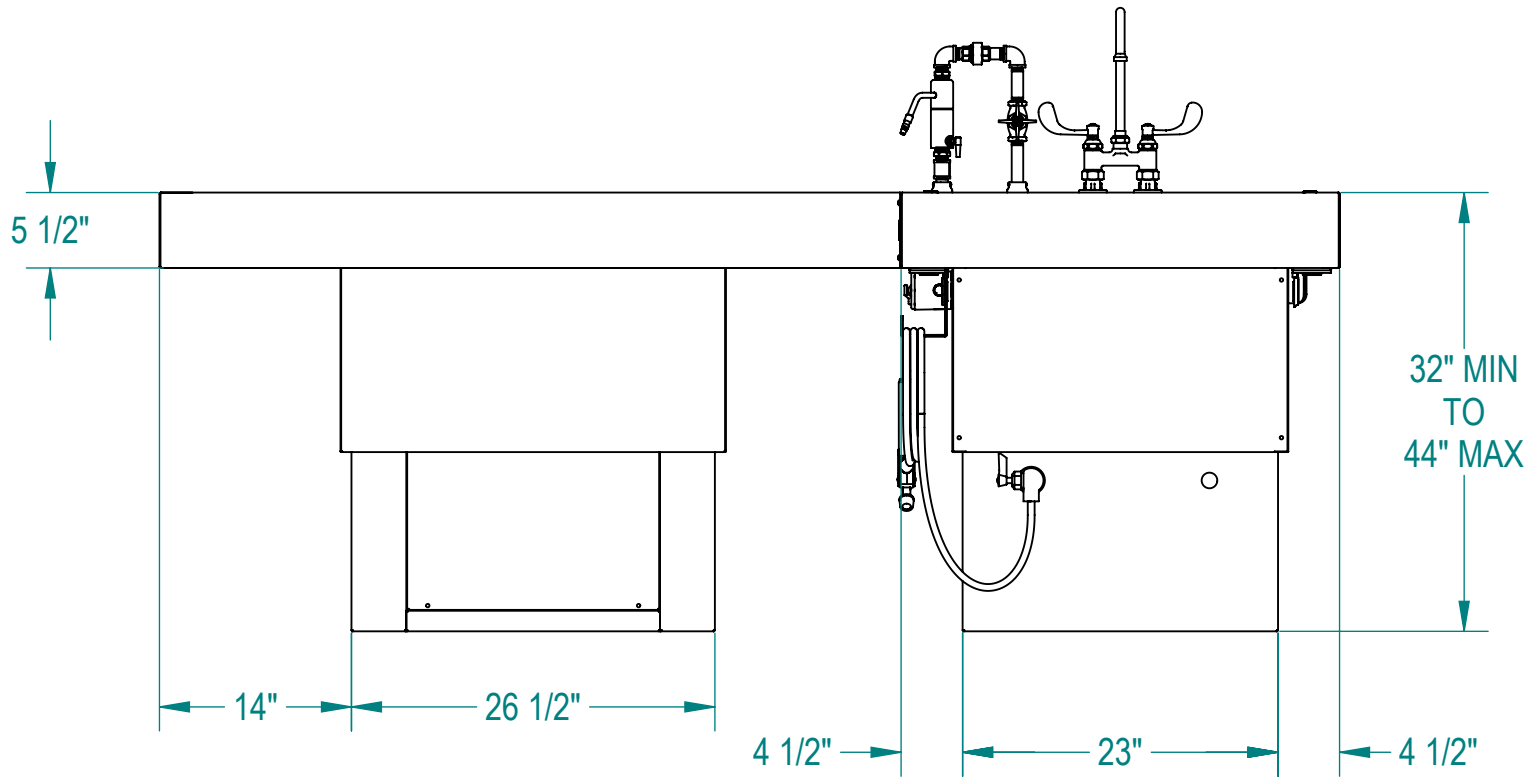


NOTES: UNLESS OTHERWISE SPECIFIED


1. APPLICABLE STANDARDS AND SPECIFICATIONS;
ASME Y14.5-2009, DIMENSIONING AND TOLERANCING
ASME Y14.5-2007, ABBREVIATIONS

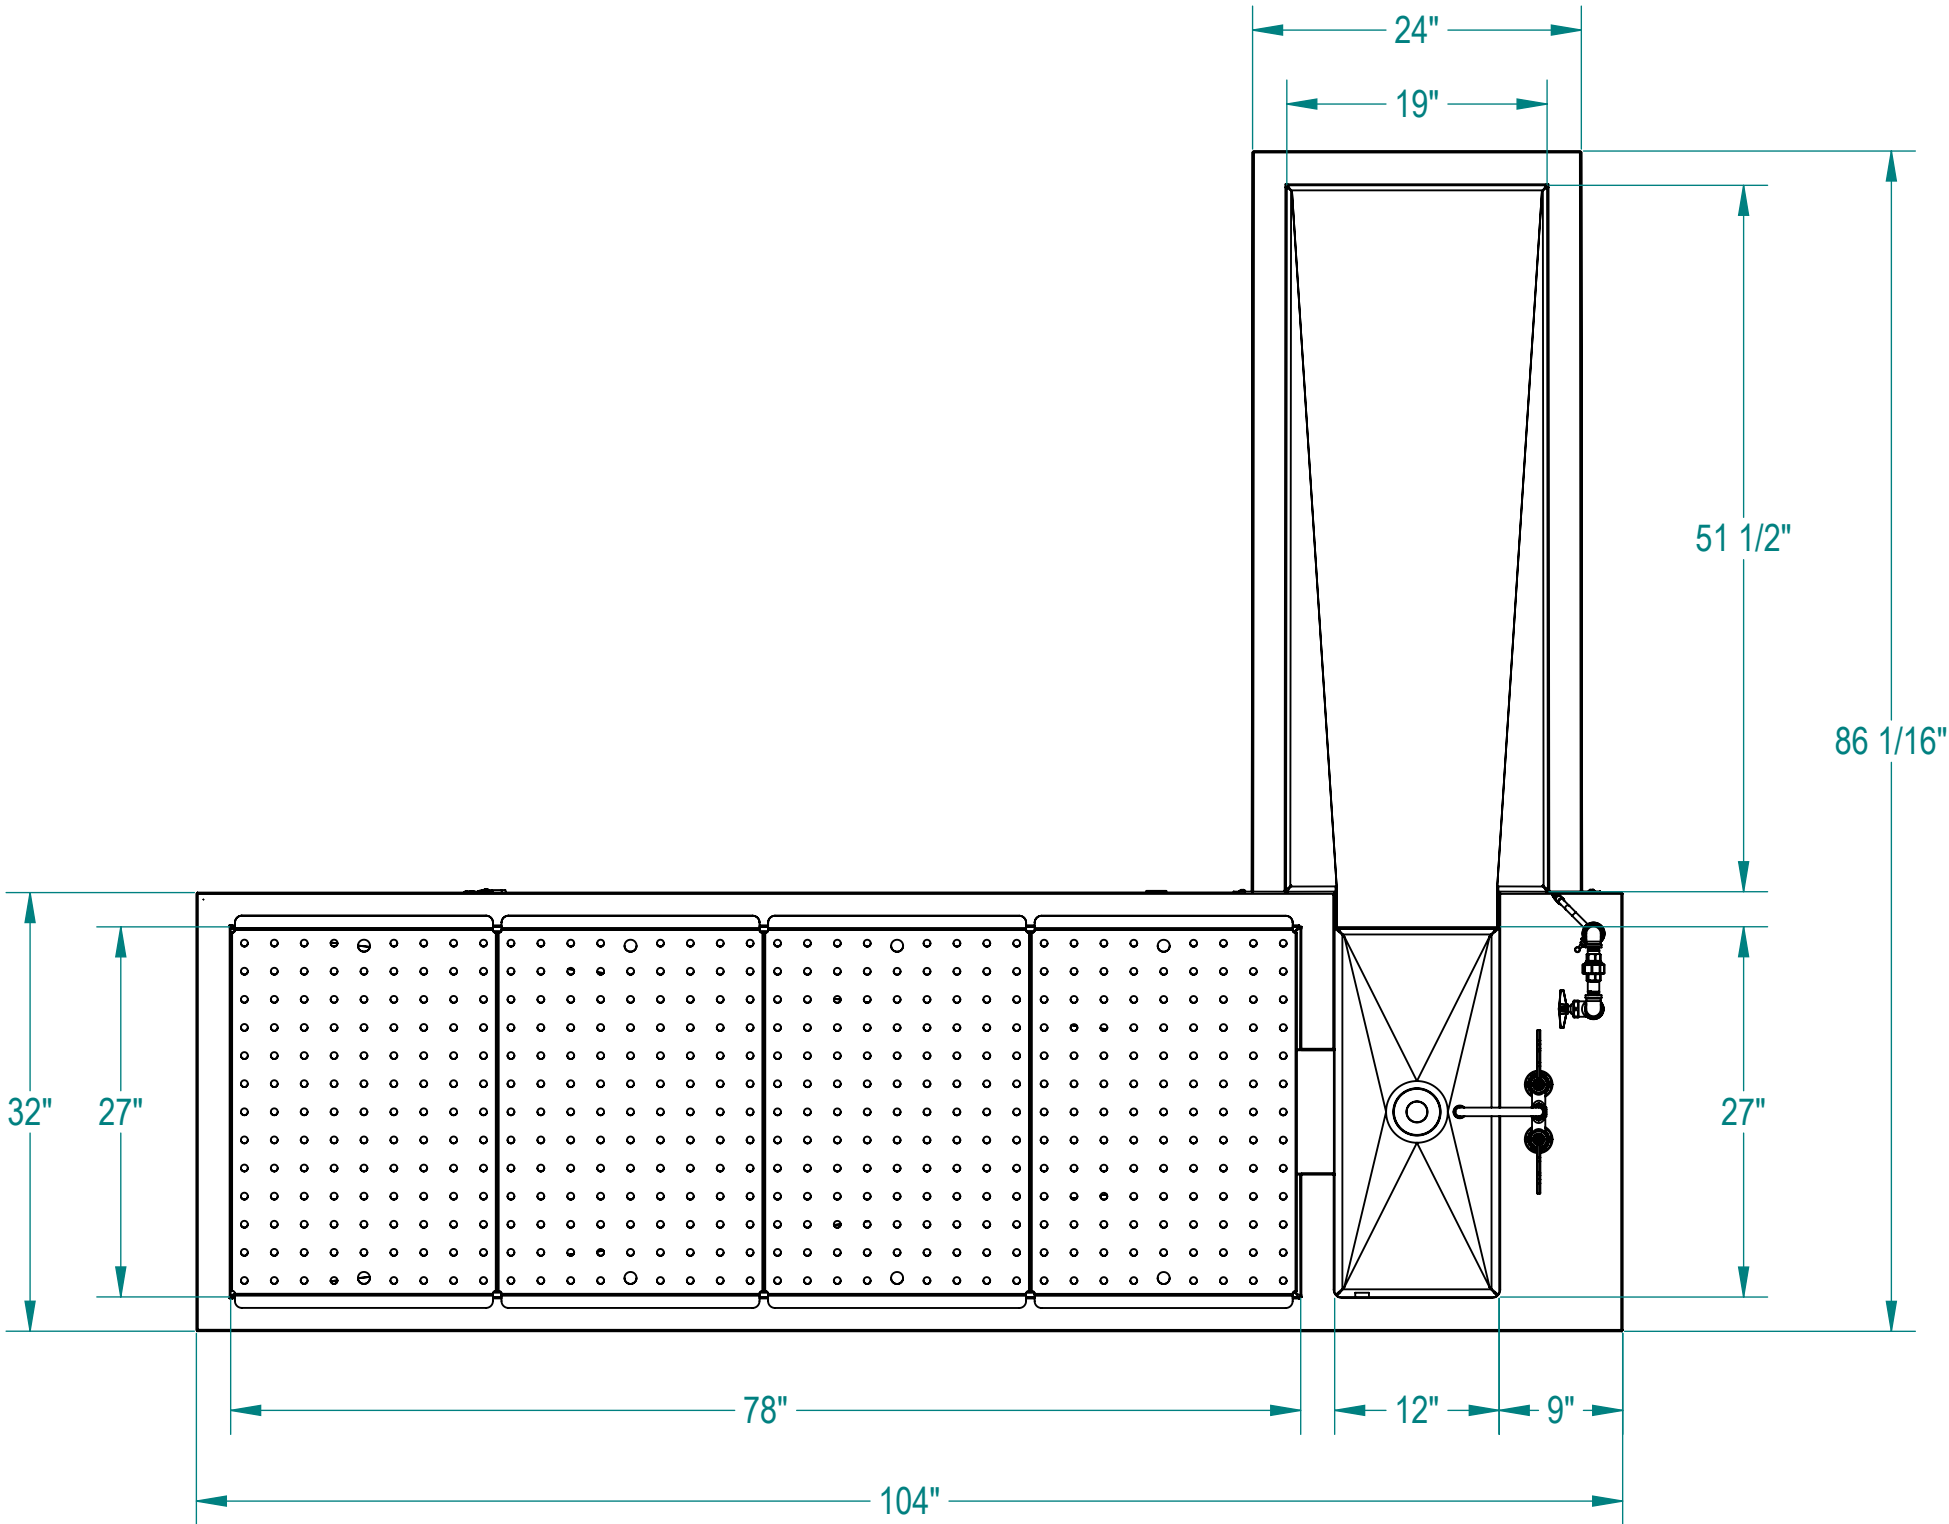

CUSTOMER		APPROVAL		PROPRIETARY THIS DOCUMENT AND THE DATE DISCLOSED HEREIN AND HEREWIT IS NOT TO BE REPRODUCED, USED, OR OTHERWISE DISCLOSED IN WHOLE OR IN PART TO ANYONE WITHOUT WRITTEN AUTHORIZATION FROM MOPEC GROUP.			   411 North Aerojet Avenue Azusa, CA 91702 tel: (800) 410-0100 (626) 334-1471 fax: (626) 334-1704 www.mopectechmfg.com				
PROJECT							TITLE MODEL 1036-19AL (CE750) PEDESTAL AUTOPSY TABLE, L-SHAPED, ADJUSTABLE HEIGHT, LEFT				
				DO NOT SCALE DRAWING		APPROVALS		DATE			
				MATERIAL		DRAWN BY		11/06/24			
				304 STAINLESS STEEL		ELISEO S.					
				FINISH		CHECKED BY					
				#4		APPROVED BY					
		SIGNATURE		DATE		SIZE		DWG NO.		REV.	
						C		1036-19AL		A	
						SCALE		NEXT ASSY.		SHEET	
						1:14				1 OF 4	

NOTES: UNLESS OTHERWISE SPECIFIED


1. APPLICABLE STANDARDS AND SPECIFICATIONS;
ASME Y14.5-2009, DIMENSIONING AND TOLERANCING
ASME Y14.5-2007, ABBREVIATIONS

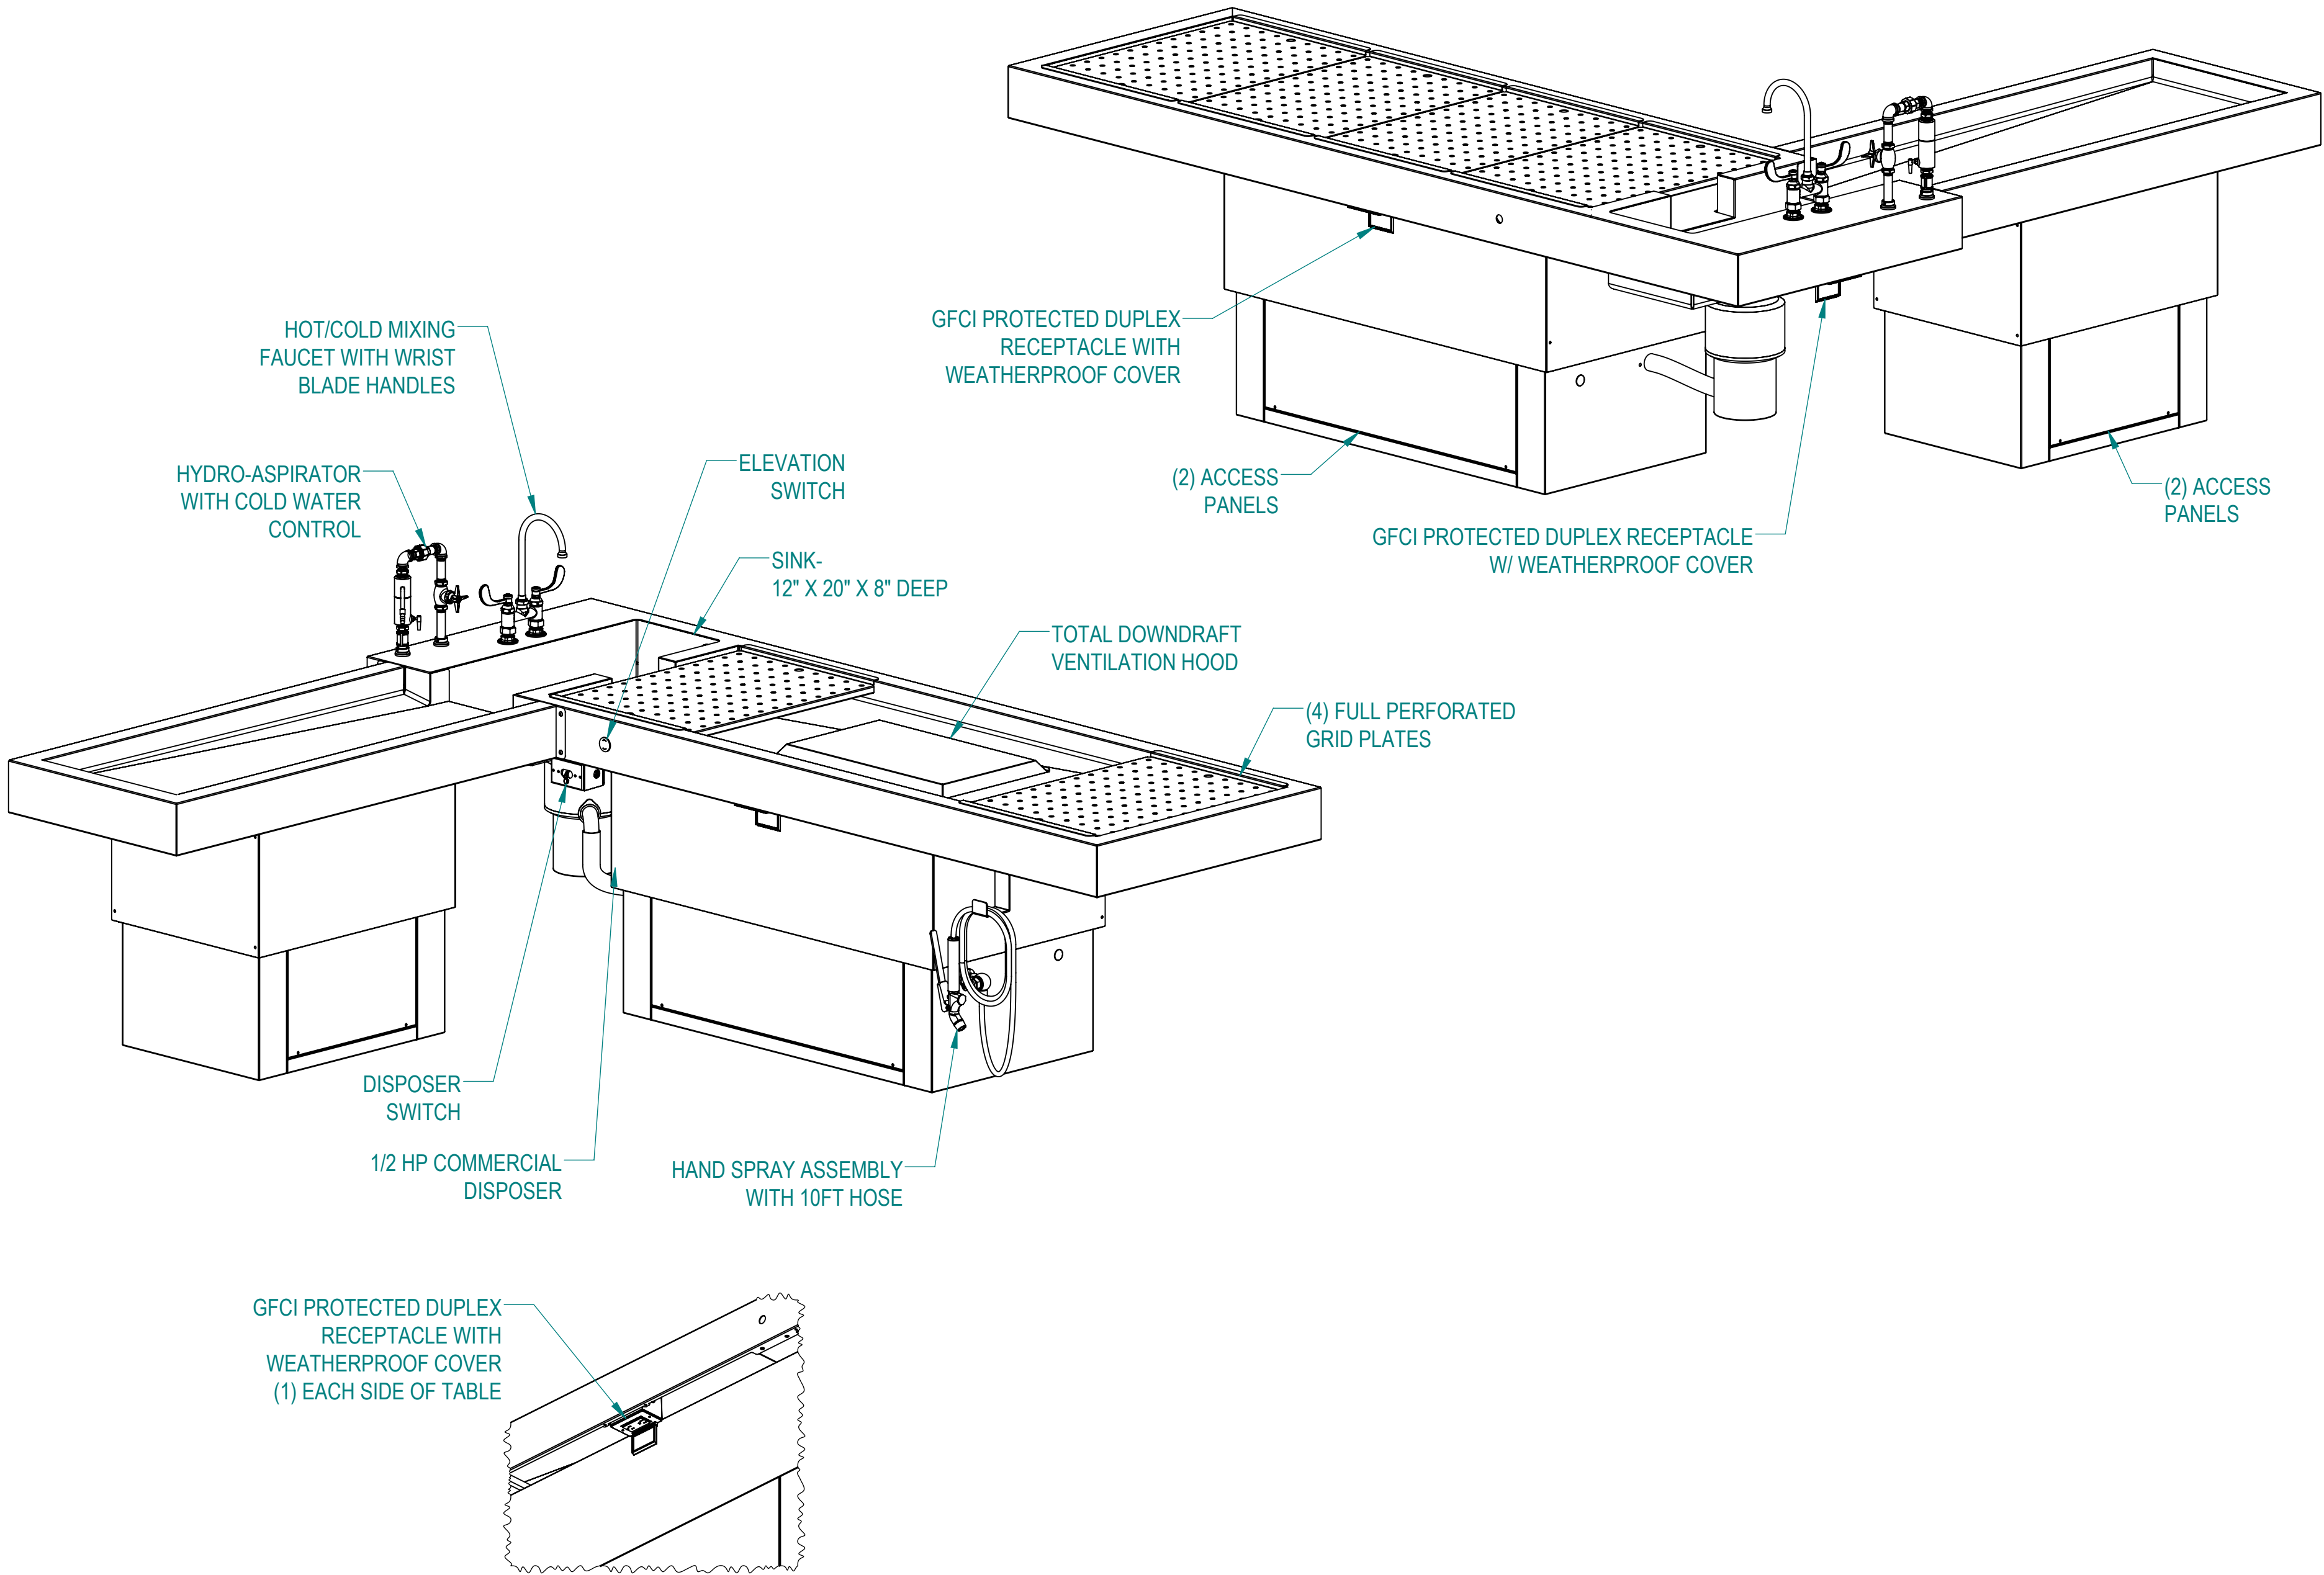

CUSTOMER		APPROVAL		PROPRIETARY THIS DOCUMENT AND THE DATE DISCLOSED HEREIN AND HEREWITH IS NOT TO BE REPRODUCED, USED, OR OTHERWISE DISCLOSED IN WHOLE OR IN PART TO ANYONE WITHOUT WRITTEN AUTHORIZATION FROM MOPEC GROUP.		 MOPEC GROUP  mopec ELEVATING PATHOLOGY  MORTECH A DIVISION OF MOPEC GROUP 411 North Aerojet Avenue Azusa, CA 91702 tel: (800) 410-0100 (626) 334-1471 fax: (626) 334-1704 www.mortechmfg.com					
PROJECT						TITLE		MODEL 1036-19AL (CE750) PEDESTAL AUTOPSY TABLE, L-SHAPED, ADJUSTABLE HEIGHT, LEFT			
		SIGNATURE		DATE		SIZE		DWG NO.		REV.	
						C		1036-19AL		A	
						SCALE		1:12		NEXT ASSY.	
								SHEET		2 OF 4	

UTILITY REQUIREMENTS:


1. A 4" X 5" AREA FOR INLET PLUMBING TO INCLUDE THE FOLLOWING:
(1) COLD WATER SUPPLY, 3/4" OD COPPER STUBBED OUT 6"
(1) HOT WATER SUPPLY, 1/2" OD COPPER STUBBED OUT 6"
SUPPLY SHUT-OFF VALVES AT EACH WATER SUPPLY
FLUSH LINES CLEAR BEFORE CONNECTING TO STATION
2. (1) STANDARD 1 1/2" WASTE LINE STUBBED OUT 6"
SUPPLY P-TRAP FOR DRAIN
3. A 4" X 4" AREA FOR ELECTRICAL INPUT TO INCLUDE THE FOLLOWING:
(1) 115V/60Hz/1PH/15A CIRCUIT FOR STATION
(1)115V/60Hz/1PH/15A CIRCUIT FOR DISPOSER
4. A 6" DIA DUCT EXHAUST CONNECTION:
RECOMMENDED EXHAUST: 450-500 CFM AT 0.50 STATIC PRESSURE
MEASURED AT THE 6" EXHAUST, PROVIDE WATER CAP OVER DUCT INLET.
EXISTING CONDITIONS MAY WARRANT AN INCREASE OR DECREASE,
CONTACT YOUR ENGINEERING DEPT.
5. PROVIDE 60-65 PSI WATER PRESSURE AND 4 GALLONS PER MINUTE OF
FLOW FOR PROPER OPERATION OF HYDRO ASPIRATOR
6. ELECTRICIAN TO PROVIDE LIQUID TIGHT JUNCTION BOX AND CONDUIT PER
LOCAL CODES.

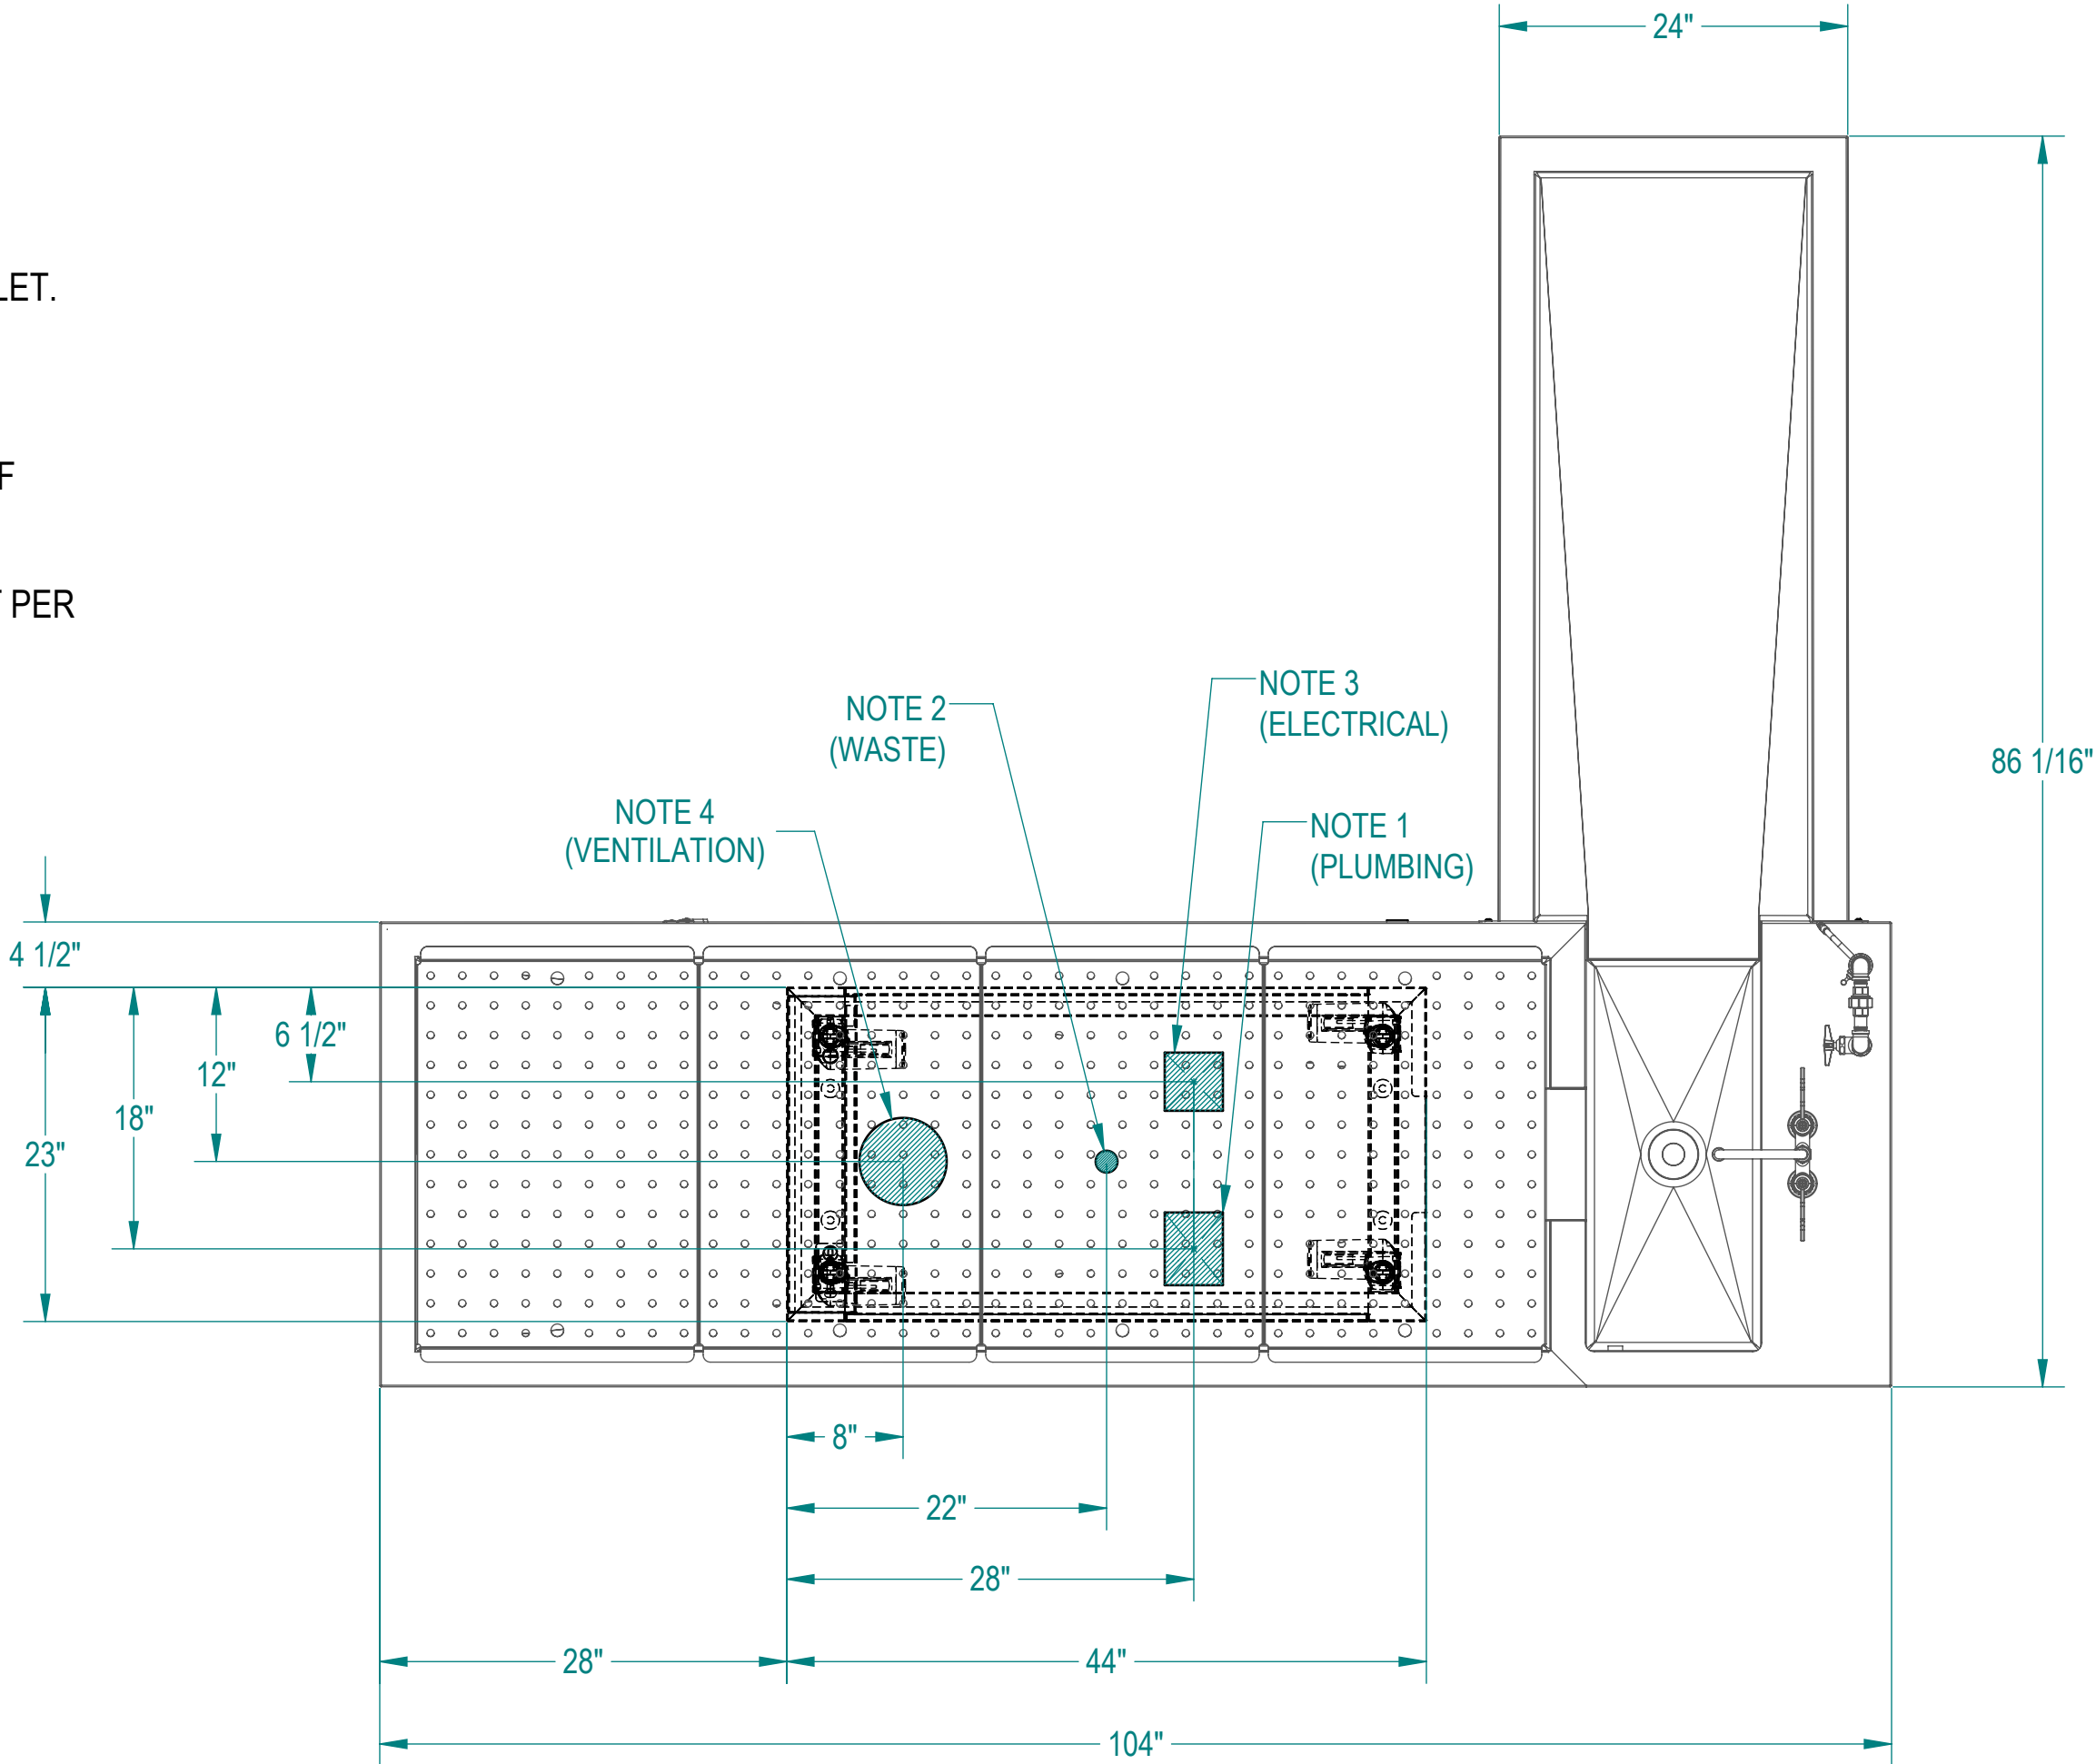

CUSTOMER		APPROVAL		PROPRIETARY THIS DOCUMENT AND THE DATE DISCLOSED HEREIN AND HEREWIT IS NOT TO BE REPRODUCED, USED, OR OTHERWISE DISCLOSED IN WHOLE OR IN PART TO ANYONE WITHOUT WRITTEN AUTHORIZATION FROM MOPEC GROUP.			MOPEC GROUP ELEVATING PATHOLOGY MORTECH MOPEC GROUP 411 North Aerojet Avenue Azusa, CA 91702 tel: (800) 410-0100 (626) 334-1471 fax: (626) 334-1704 www.mopecgroup.com				
PROJECT							TITLE MODEL 1036-19AL (CE750) PEDESTAL AUTOPSY TABLE, L-SHAPED, ADJUSTABLE HEIGHT, LEFT				
				DO NOT SCALE DRAWING		APPROVALS		DATE			
				MATERIAL		DRAWN BY		11/06/24			
				304 STAINLESS STEEL		ELISEO S.					
				FINISH		CHECKED BY					
				#4		APPROVED BY					

NOTES: UNLESS OTHERWISE SPECIFIED

1.
- APPLICABLE STANDARDS AND SPECIFICATIONS;
ASME Y14.5-2009, DIMENSIONING AND TOLERANCING
ASME Y14.5-2007, ABBREVIATIONS

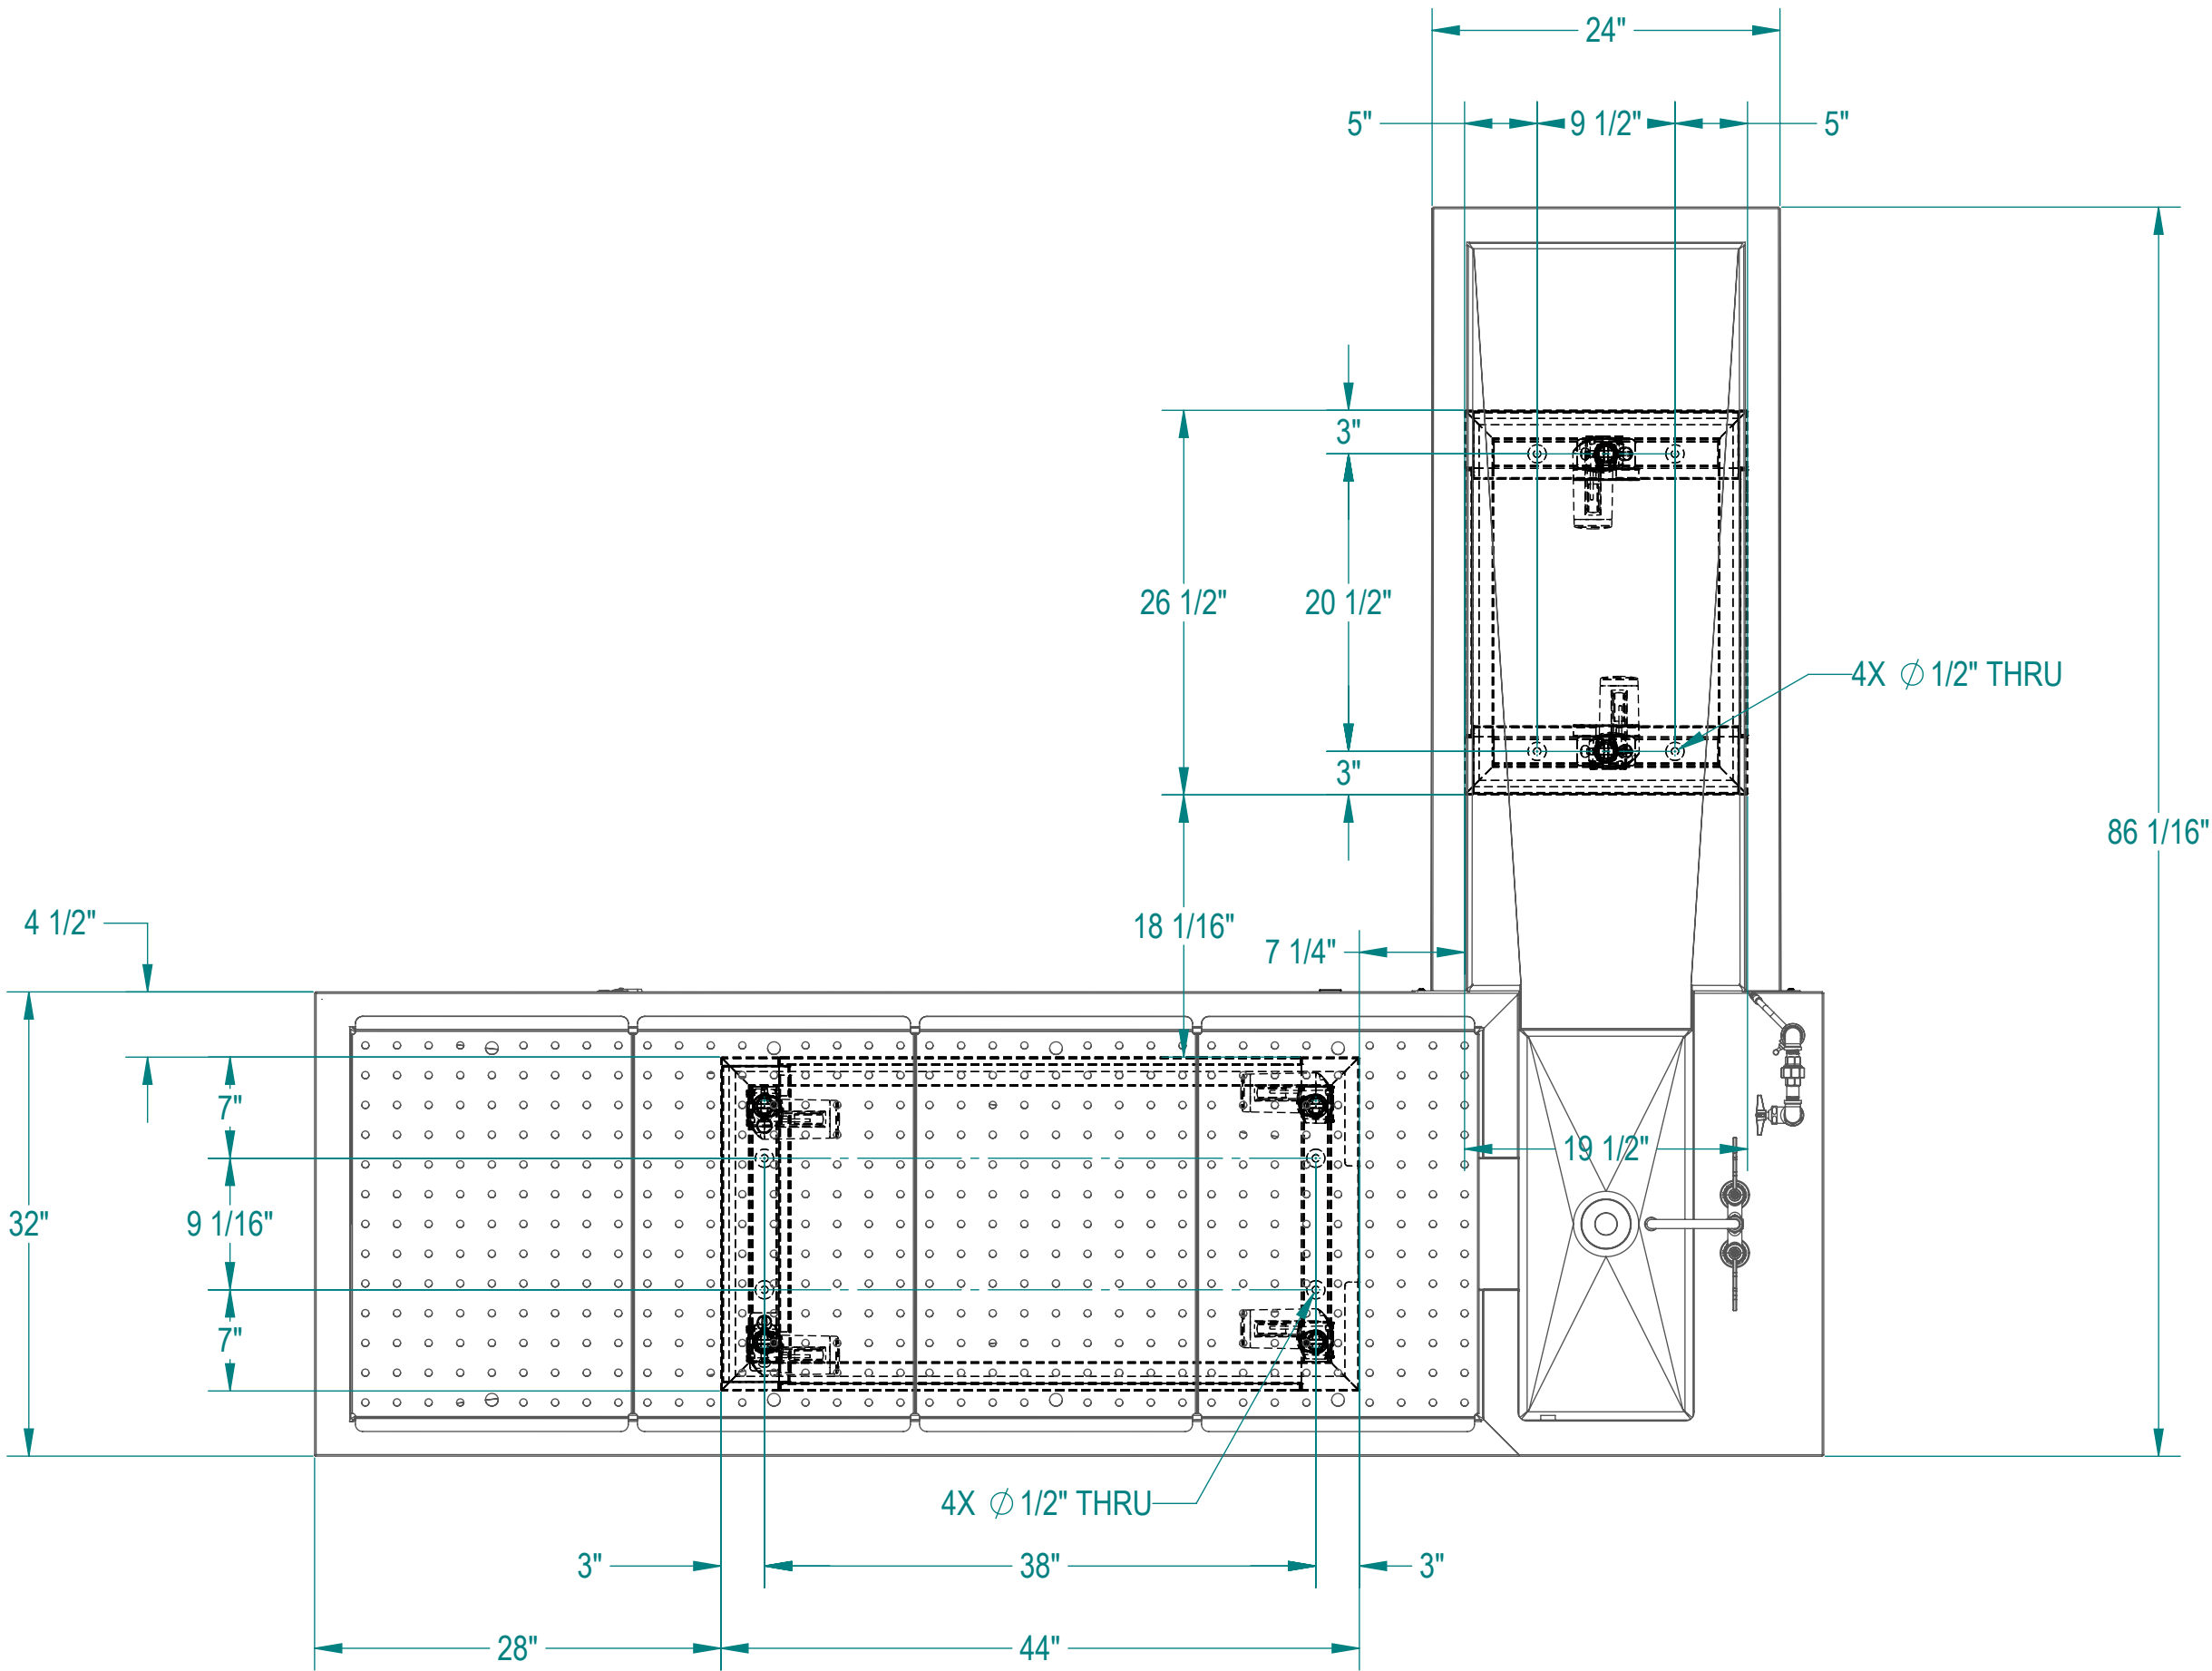

FLOOR MOUNTING
DETAIL

CUSTOMER	APPROVAL		PROPRIETARY THIS DOCUMENT AND THE DATE DISCLOSED HEREIN AND HEREWIT IS NOT TO BE REPRODUCED, USED, OR OTHERWISE DISCLOSED IN WHOLE OR IN PART TO ANYONE WITHOUT WRITTEN AUTHORIZATION FROM MOPEC GROUP.			MOPEC GROUP Mopec ELEVATING PATHOLOGY MORTECH MEMBER OF MOPEC GROUP 411 North Aerojet Avenue Azusa, CA 91702 tel: (800) 410-0100 (626) 334-1471 fax: (626) 334-1704 www.mopectechmfg.com		
PROJECT						TITLE MODEL 1036-19AL (CE750) PEDESTAL AUTOPSY TABLE, L-SHAPED, ADJUSTABLE HEIGHT, LEFT		
SIGNATUREDATE			DO NOT SCALE DRAWING		APPROVALS	DATE	SIZEDWG NO. 1036-19AL REV. A	
			MATERIAL 304 STAINLESS STEEL		DRAWN BY ELISEO S.	11/06/24		
			FINISH #4		CHECKED BY			
					APPROVED BY			
					SCALE	1:12	NEXT ASSY.	SHEET 4 OF 4