
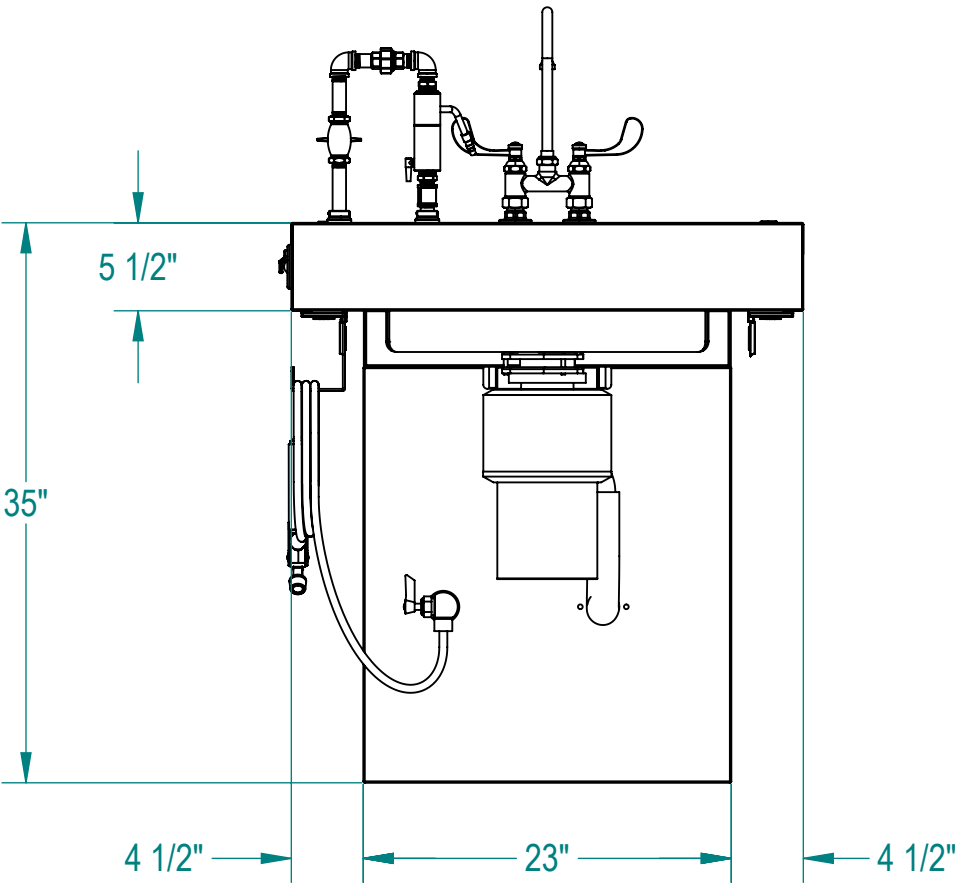
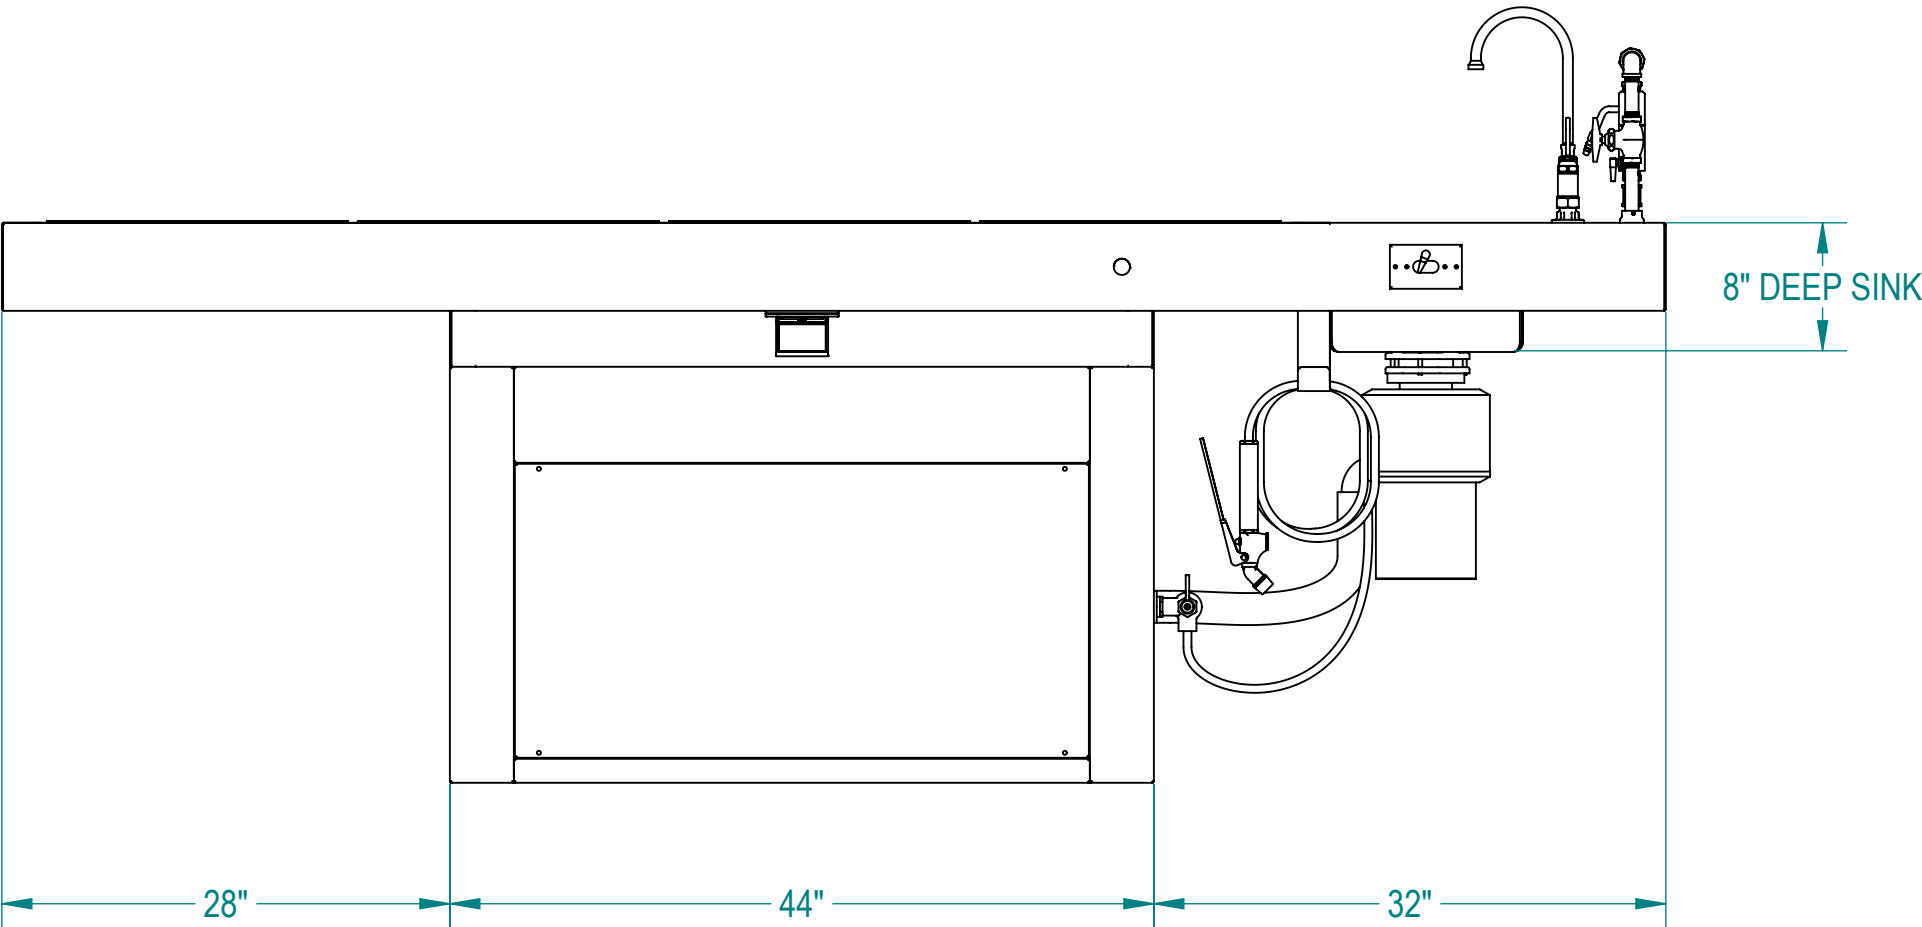


NOTES: UNLESS OTHERWISE SPECIFIED


1. APPLICABLE STANDARDS AND SPECIFICATIONS;
- ASME Y14.5-2009, DIMENSIONING AND TOLERANCING
- ASME Y14.5-2007, ABBREVIATIONS

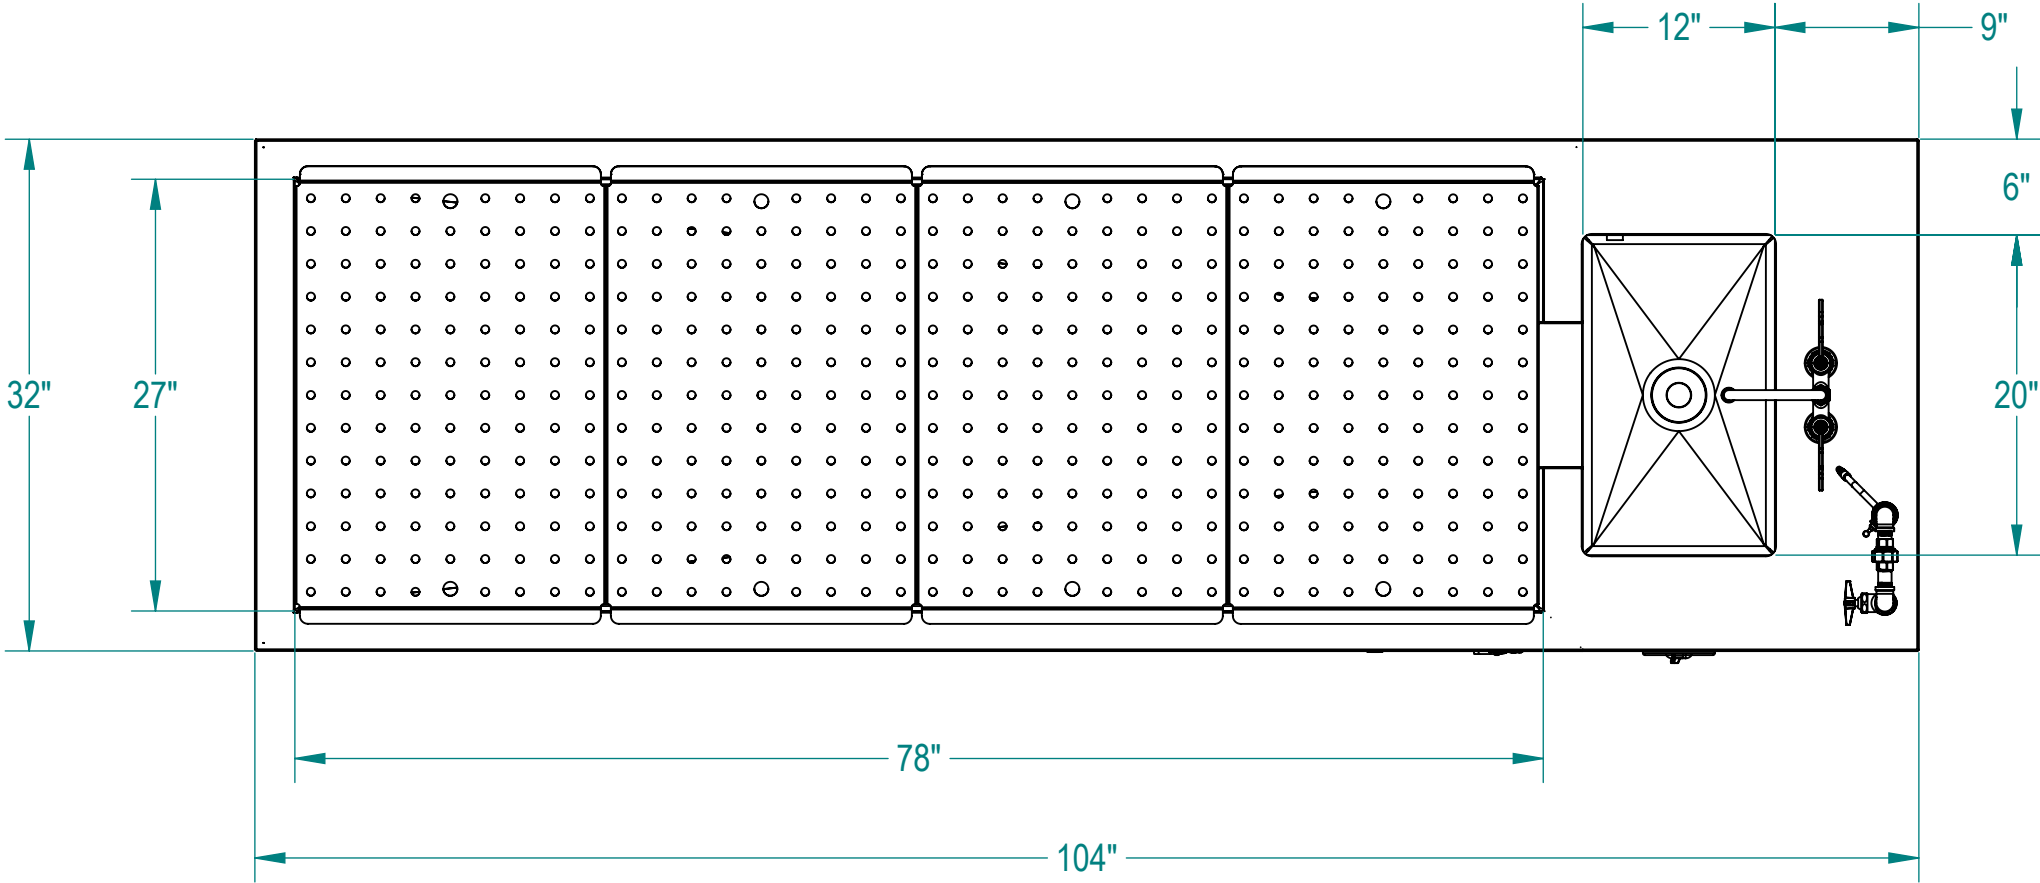

CUSTOMER		APPROVAL		<div>PROPRIETARY</div> <div>THIS DOCUMENT AND THE DATE DISCLOSED HEREIN AND HEREWITH IS NOT TO BE REPRODUCED, USED, OR OTHERWISE DISCLOSED IN WHOLE OR IN PART TO ANYONE WITHOUT WRITTEN AUTHORIZATION FROM MOPEC GROUP.</div>			<div><div>MOPEC</div><div>GROUP</div></div> <div><div>Mopec</div><div>ELEVATING PATHOLOGY</div><div>MORTECH</div><div><small>A DIVISION OF MOPEC GROUP</small></div></div>		
PROJECT						TITLE			
						MODEL 1036-41-TD (CE100)			
						PEDESTAL AUTOPSY TABLE, VENTED			
SIGNATURE		DATE		DO NOT SCALE DRAWING		APPROVALS		DATE	
				MATERIAL		DRAWN BY		10/10/24	
				304 STAINLESS STEEL		ELISEO S.			
				FINISH		CHECKED BY			
				#4		APPROVED BY			
								SCALE	
								1:12	
								NEXT ASSY.	
								SHEET	
								1 OF 3	
								REV.	
								A	

NOTES: UNLESS OTHERWISE SPECIFIED



1. APPLICABLE STANDARDS AND SPECIFICATIONS;
ASME Y14.5-2009, DIMENSIONING AND TOLERANCING
ASME Y14.5-2007, ABBREVIATIONS

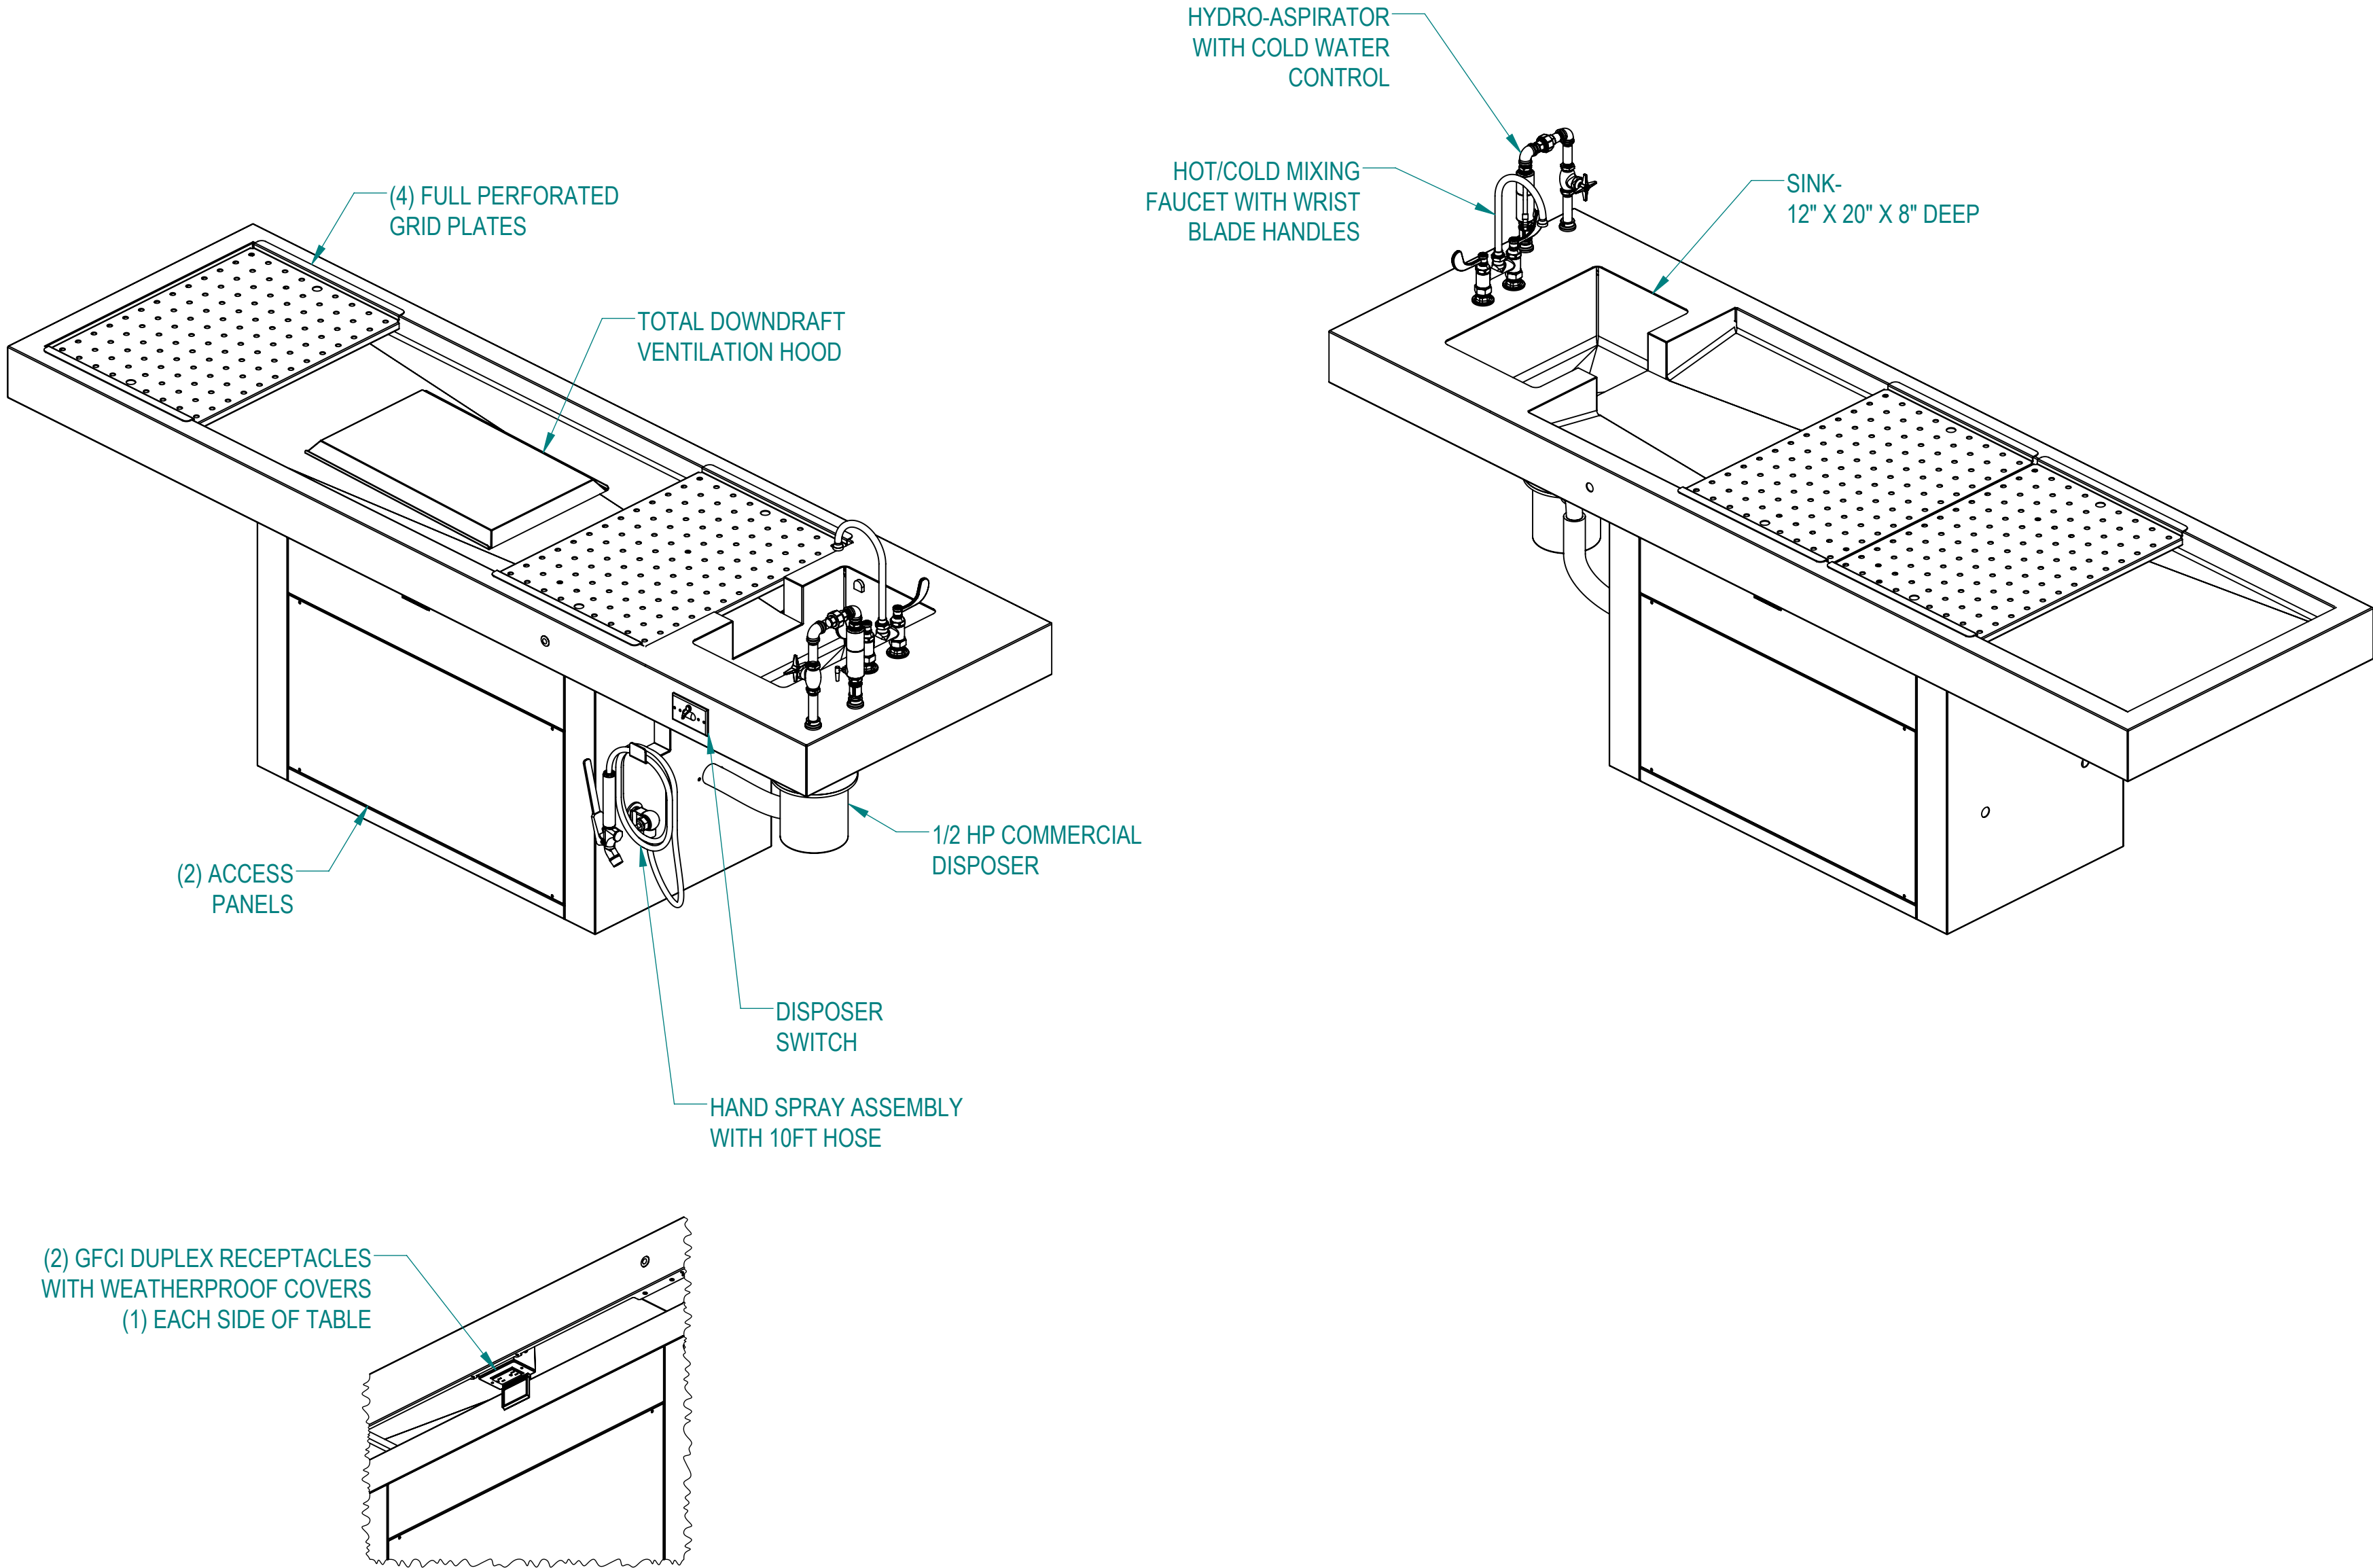

CUSTOMER		APPROVAL		PROPRIETARY		MOPEC GROUP		MORTECH	
PROJECT				THIS DOCUMENT AND THE DATE DISCLOSED HEREIN AND HERewith IS NOT TO BE REPRODUCED, USED, OR OTHERWISE DISCLOSED IN WHOLE OR IN PART TO ANYONE WITHOUT WRITTEN AUTHORIZATION FROM MOPEC GROUP.		TITLE		MODEL 1036-41-TD (CE100)	
				DO NOT SCALE DRAWING		APPROVALS		DATE	
				MATERIAL		DRAWN BY		10/10/24	
				304 STAINLESS STEEL		CHECKED BY			
				FINISH		APPROVED BY			
				#4					
						SIZE		DWG NO.	
						C		1036-41-TD	
						SCALE		NEXT ASSY.	
						1:12		SHEET	
						2		OF	
								3	
								REV.	
								A	

UTILITY REQUIREMENTS:

1. A 4" X 5" AREA FOR INLET PLUMBING TO INCLUDE THE FOLLOWING:
(1) COLD WATER SUPPLY, 3/4" OD COPPER STUBBED OUT 6"
(1) HOT WATER SUPPLY, 1/2" OD COPPER STUBBED OUT 6"
SUPPLY SHUT-OFF VALVES AT EACH WATER SUPPLY
FLUSH LINES CLEAR BEFORE CONNECTING TO STATION
2. (1) STANDARD 1 1/2" WASTE LINE STUBBED OUT 6"
SUPPLY P-TRAP FOR DRAIN
3. A 4" X 4" AREA FOR ELECTRICAL INPUT TO INCLUDE THE FOLLOWING:
(1) 115V/60Hz/1PH/15A CIRCUIT FOR STATION
(1)115V/60Hz/1PH/15A CIRCUIT FOR DISPOSER
4. A 6" DIA DUCT EXHAUST CONNECTION:
RECOMMENDED EXHAUST: 450-500 CFM AT 0.50 STATIC PRESSURE
MEASURED AT THE 6" EXHAUST, PROVIDE WATER CAP OVER DUCT INLET.
EXISTING CONDITIONS MAY WARRANT AN INCREASE OR DECREASE,
CONTACT YOUR ENGINEERING DEPT.
5. PROVIDE 60-65 PSI WATER PRESSURE AND 4 GALLONS PER MINUTE OF
FLOW FOR PROPER OPERATION OF HYDRO ASPIRATOR
6. ELECTRICIAN TO PROVIDE LIQUID TIGHT JUNCTION BOX AND CONDUIT PER
LOCAL CODES.

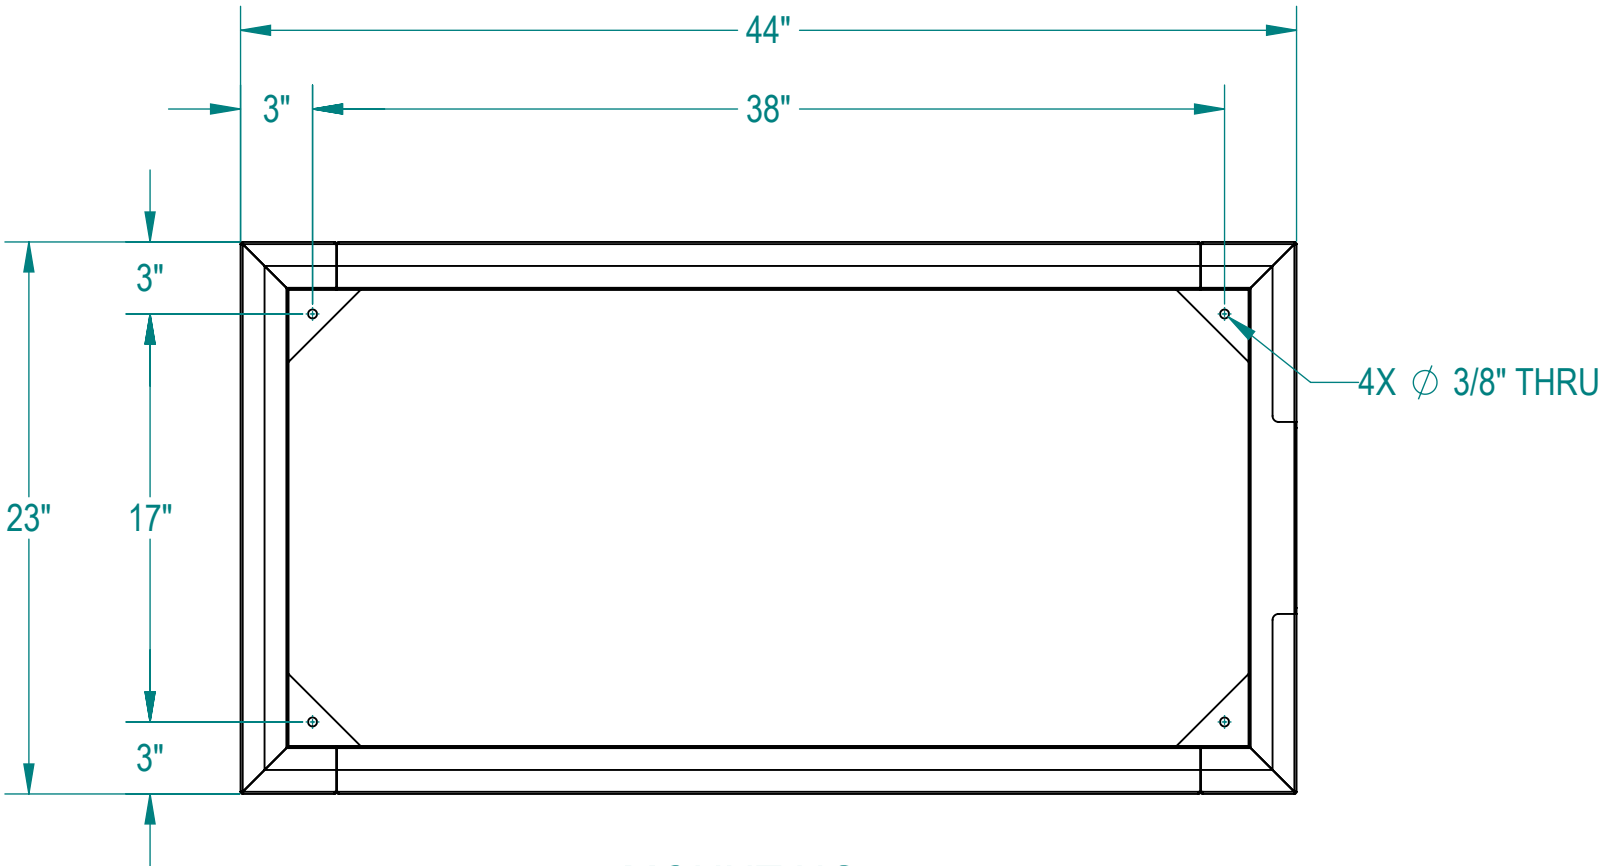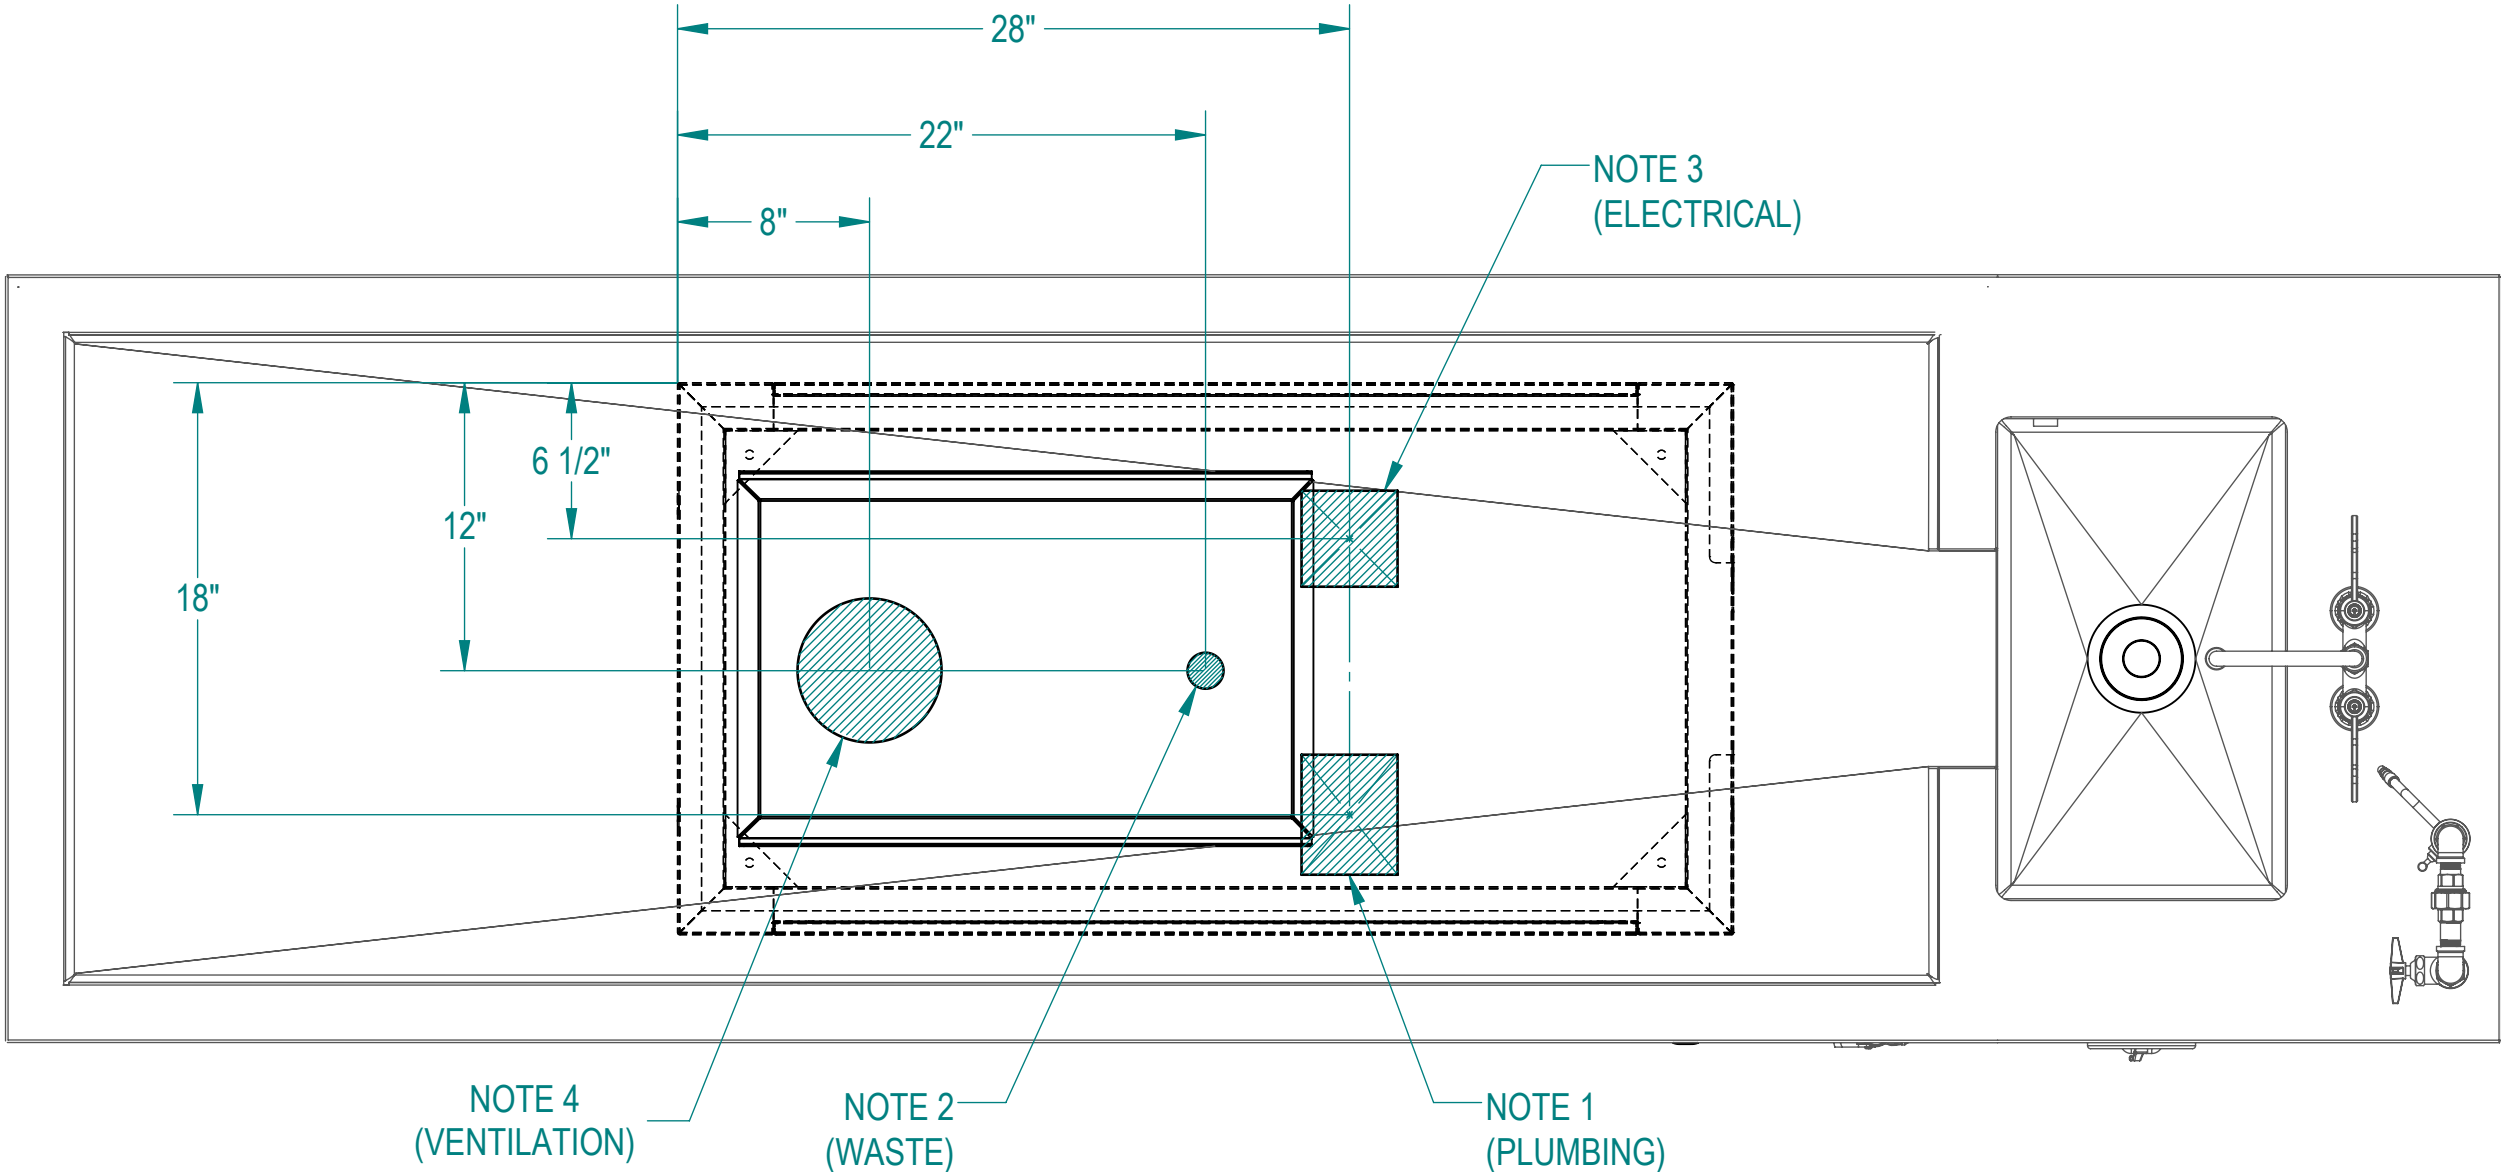

CUSTOMER	APPROVAL		<div>PROPRIETARY</div> <div>THIS DOCUMENT AND THE DATE DISCLOSED HEREIN AND HEREWIT IS NOT TO BE REPRODUCED, USED, OR OTHERWISE DISCLOSED IN WHOLE OR IN PART TO ANYONE WITHOUT WRITTEN AUTHORIZATION FROM MOPEC GROUP.</div>			<div><div><div>MOPEC</div><div>GROUP</div></div><div><div><div>Mopec</div><div>ELEVATING PATHOLOGY</div></div><div><div>MORTECH</div><div>A DIVISION OF MOPEC GROUP</div></div></div></div>		<div>TITLE</div> <div><div>MODEL 1036-41-TD (CE100)</div><div>PEDESTAL AUTOPSY TABLE, VENTED</div></div>											
PROJECT						<div>DO NOT SCALE DRAWING</div> <div>APPROVALS</div> <div>DATE</div>													
	SIGNATURE	DATE	MATERIAL		DRAWN BY		10/10/24		SIZE		DWG NO.		REV.						
			304 STAINLESS STEEL		ELISEO S.		CHECKED BY		C		1036-41-TD		A						
			FINISH		#4		APPROVED BY		SCALE		1:8		NEXT ASSY.		SHEET		3		OF