
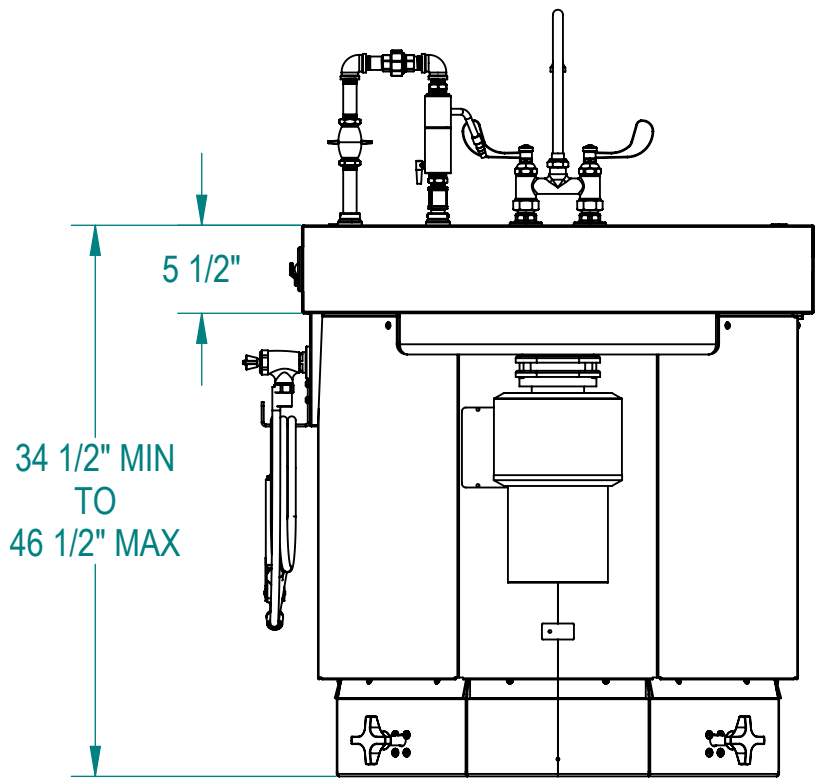
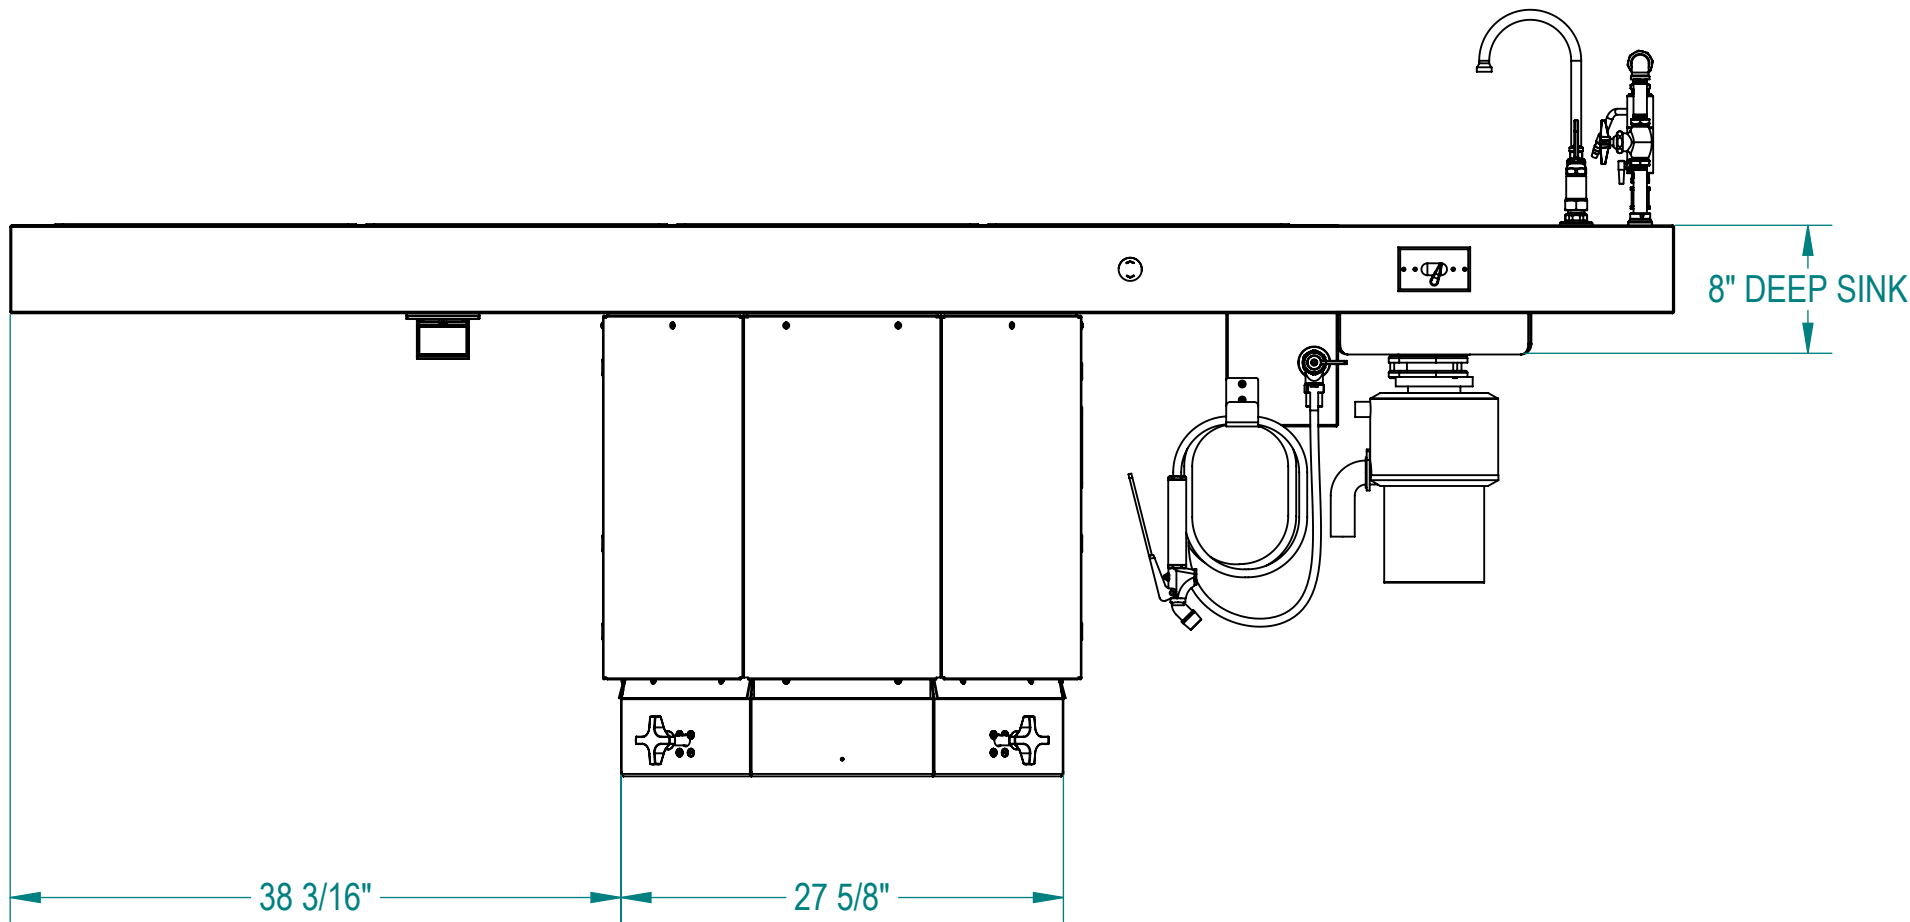


NOTES: UNLESS OTHERWISE SPECIFIED


1. APPLICABLE STANDARDS AND SPECIFICATIONS;
ASME Y14.5-2009, DIMENSIONING AND TOLERANCING
ASME Y14.5-2007, ABBREVIATIONS

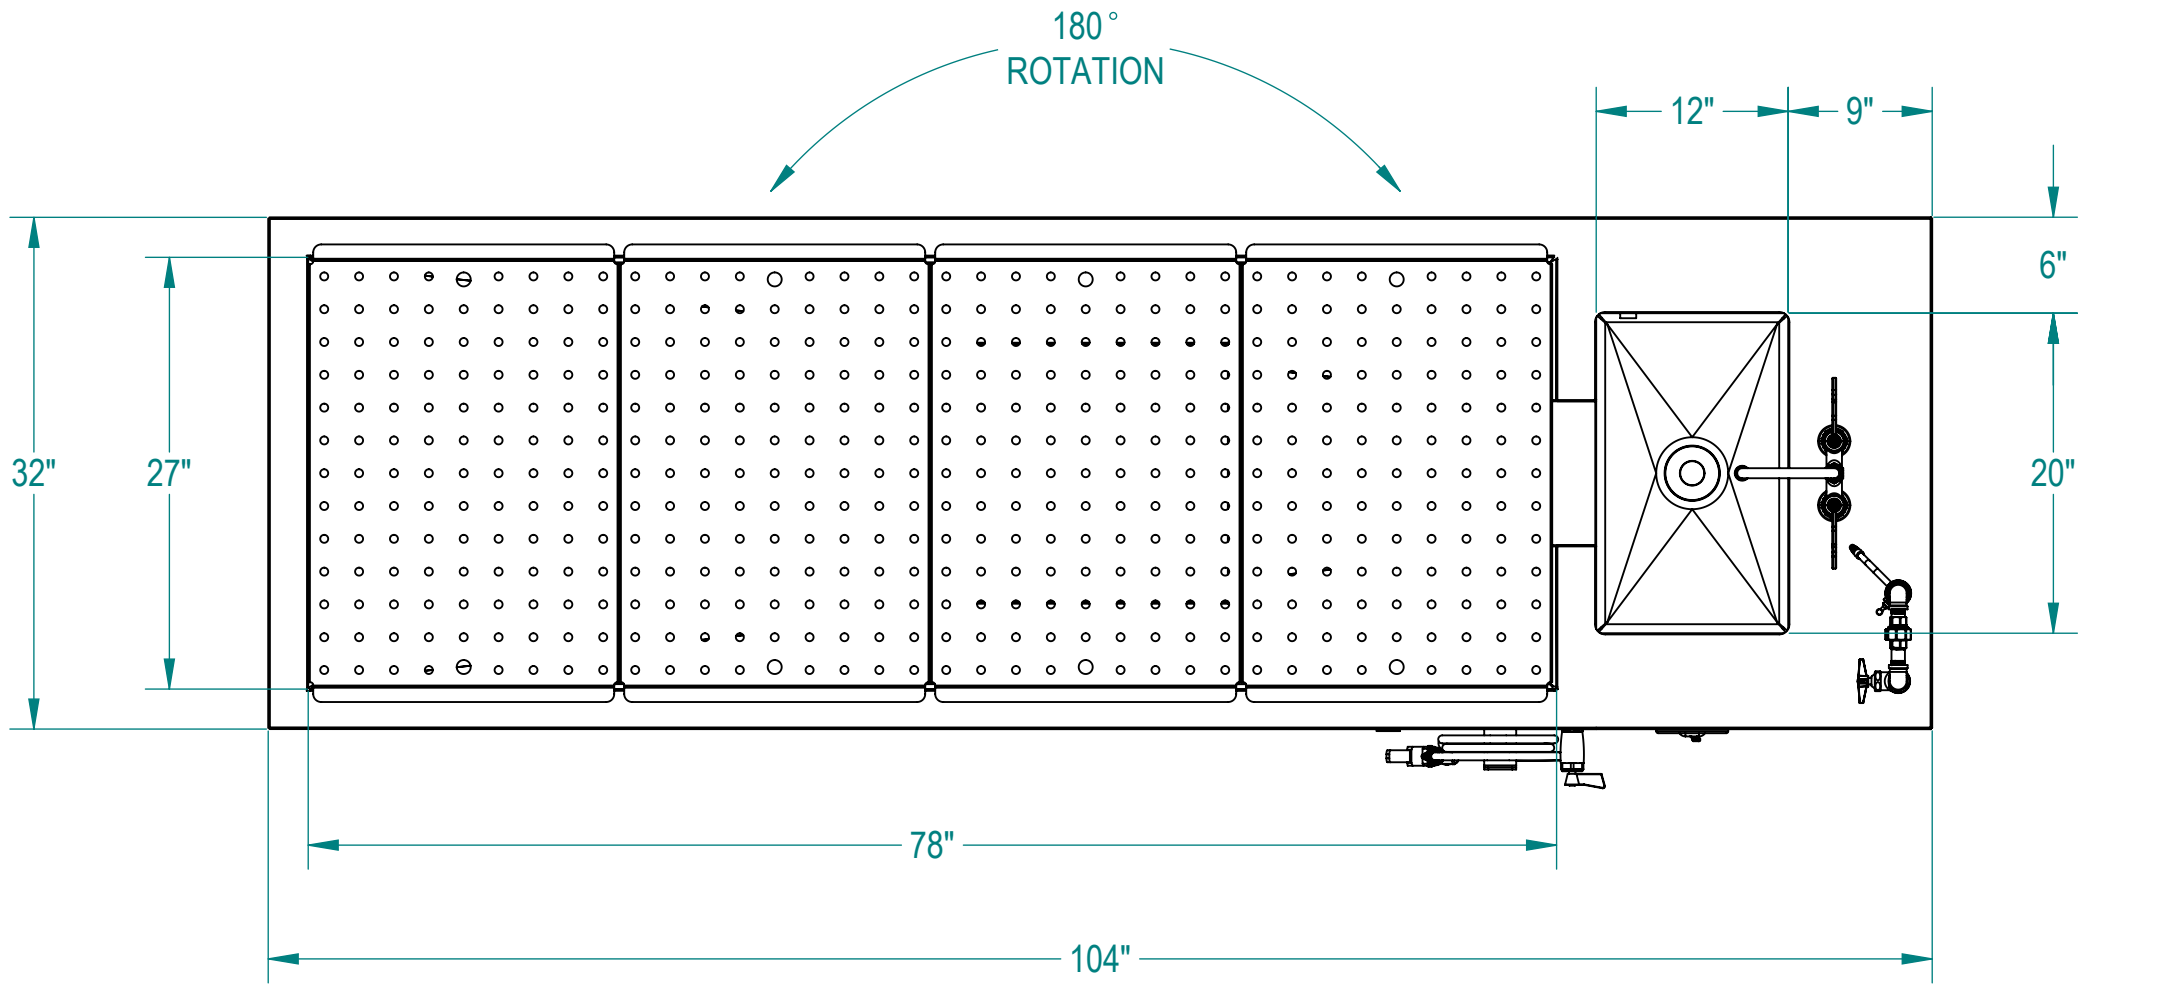

CUSTOMER		APPROVAL		<div>PROPRIETARY</div> <div>THIS DOCUMENT AND THE DATE DISCLOSED HEREIN AND HEREWIT IS NOT TO BE REPRODUCED, USED, OR OTHERWISE DISCLOSED IN WHOLE OR IN PART TO ANYONE WITHOUT WRITTEN AUTHORIZATION FROM MOPEC GROUP.</div>		<div><div><div>MOPEC</div><div>GROUP</div></div><div><div>Mopec</div><div>ELEVATING PATHOLOGY</div><div>MORTECH</div><div><small>DIVISION OF MOPEC GROUP</small></div></div></div> <div><div>411 North Aerojet Avenue Azusa, CA 91702</div><div>tel: (800) 410-0100 (626) 334-1471 fax: (626) 334-1704 www.mopectechmfg.com</div></div>					
PROJECT						TITLE <div>MODEL 1036-48-MG (CE310)</div> <div>PEDESTAL AUTOPSY TABLE, ELEVATING & ROTATING</div>					
						MATERIAL		DRAWN BY		DATE	
						304 STAINLESS STEEL		ELISEO S.		03/27/25	
		SIGNATURE		DATE		CHECKED BY					
						FINISH		APPROVED BY			
				#4							
						SIZE		DWG NO.			
						C		1036-48-MG			
						SCALE		1:12			
						NEXT ASSY.					
						SHEET		1 OF 3			

NOTES: UNLESS OTHERWISE SPECIFIED

1. APPLICABLE STANDARDS AND SPECIFICATIONS;
ASME Y14.5-2009, DIMENSIONING AND TOLERANCING
ASME Y14.5-2007, ABBREVIATIONS

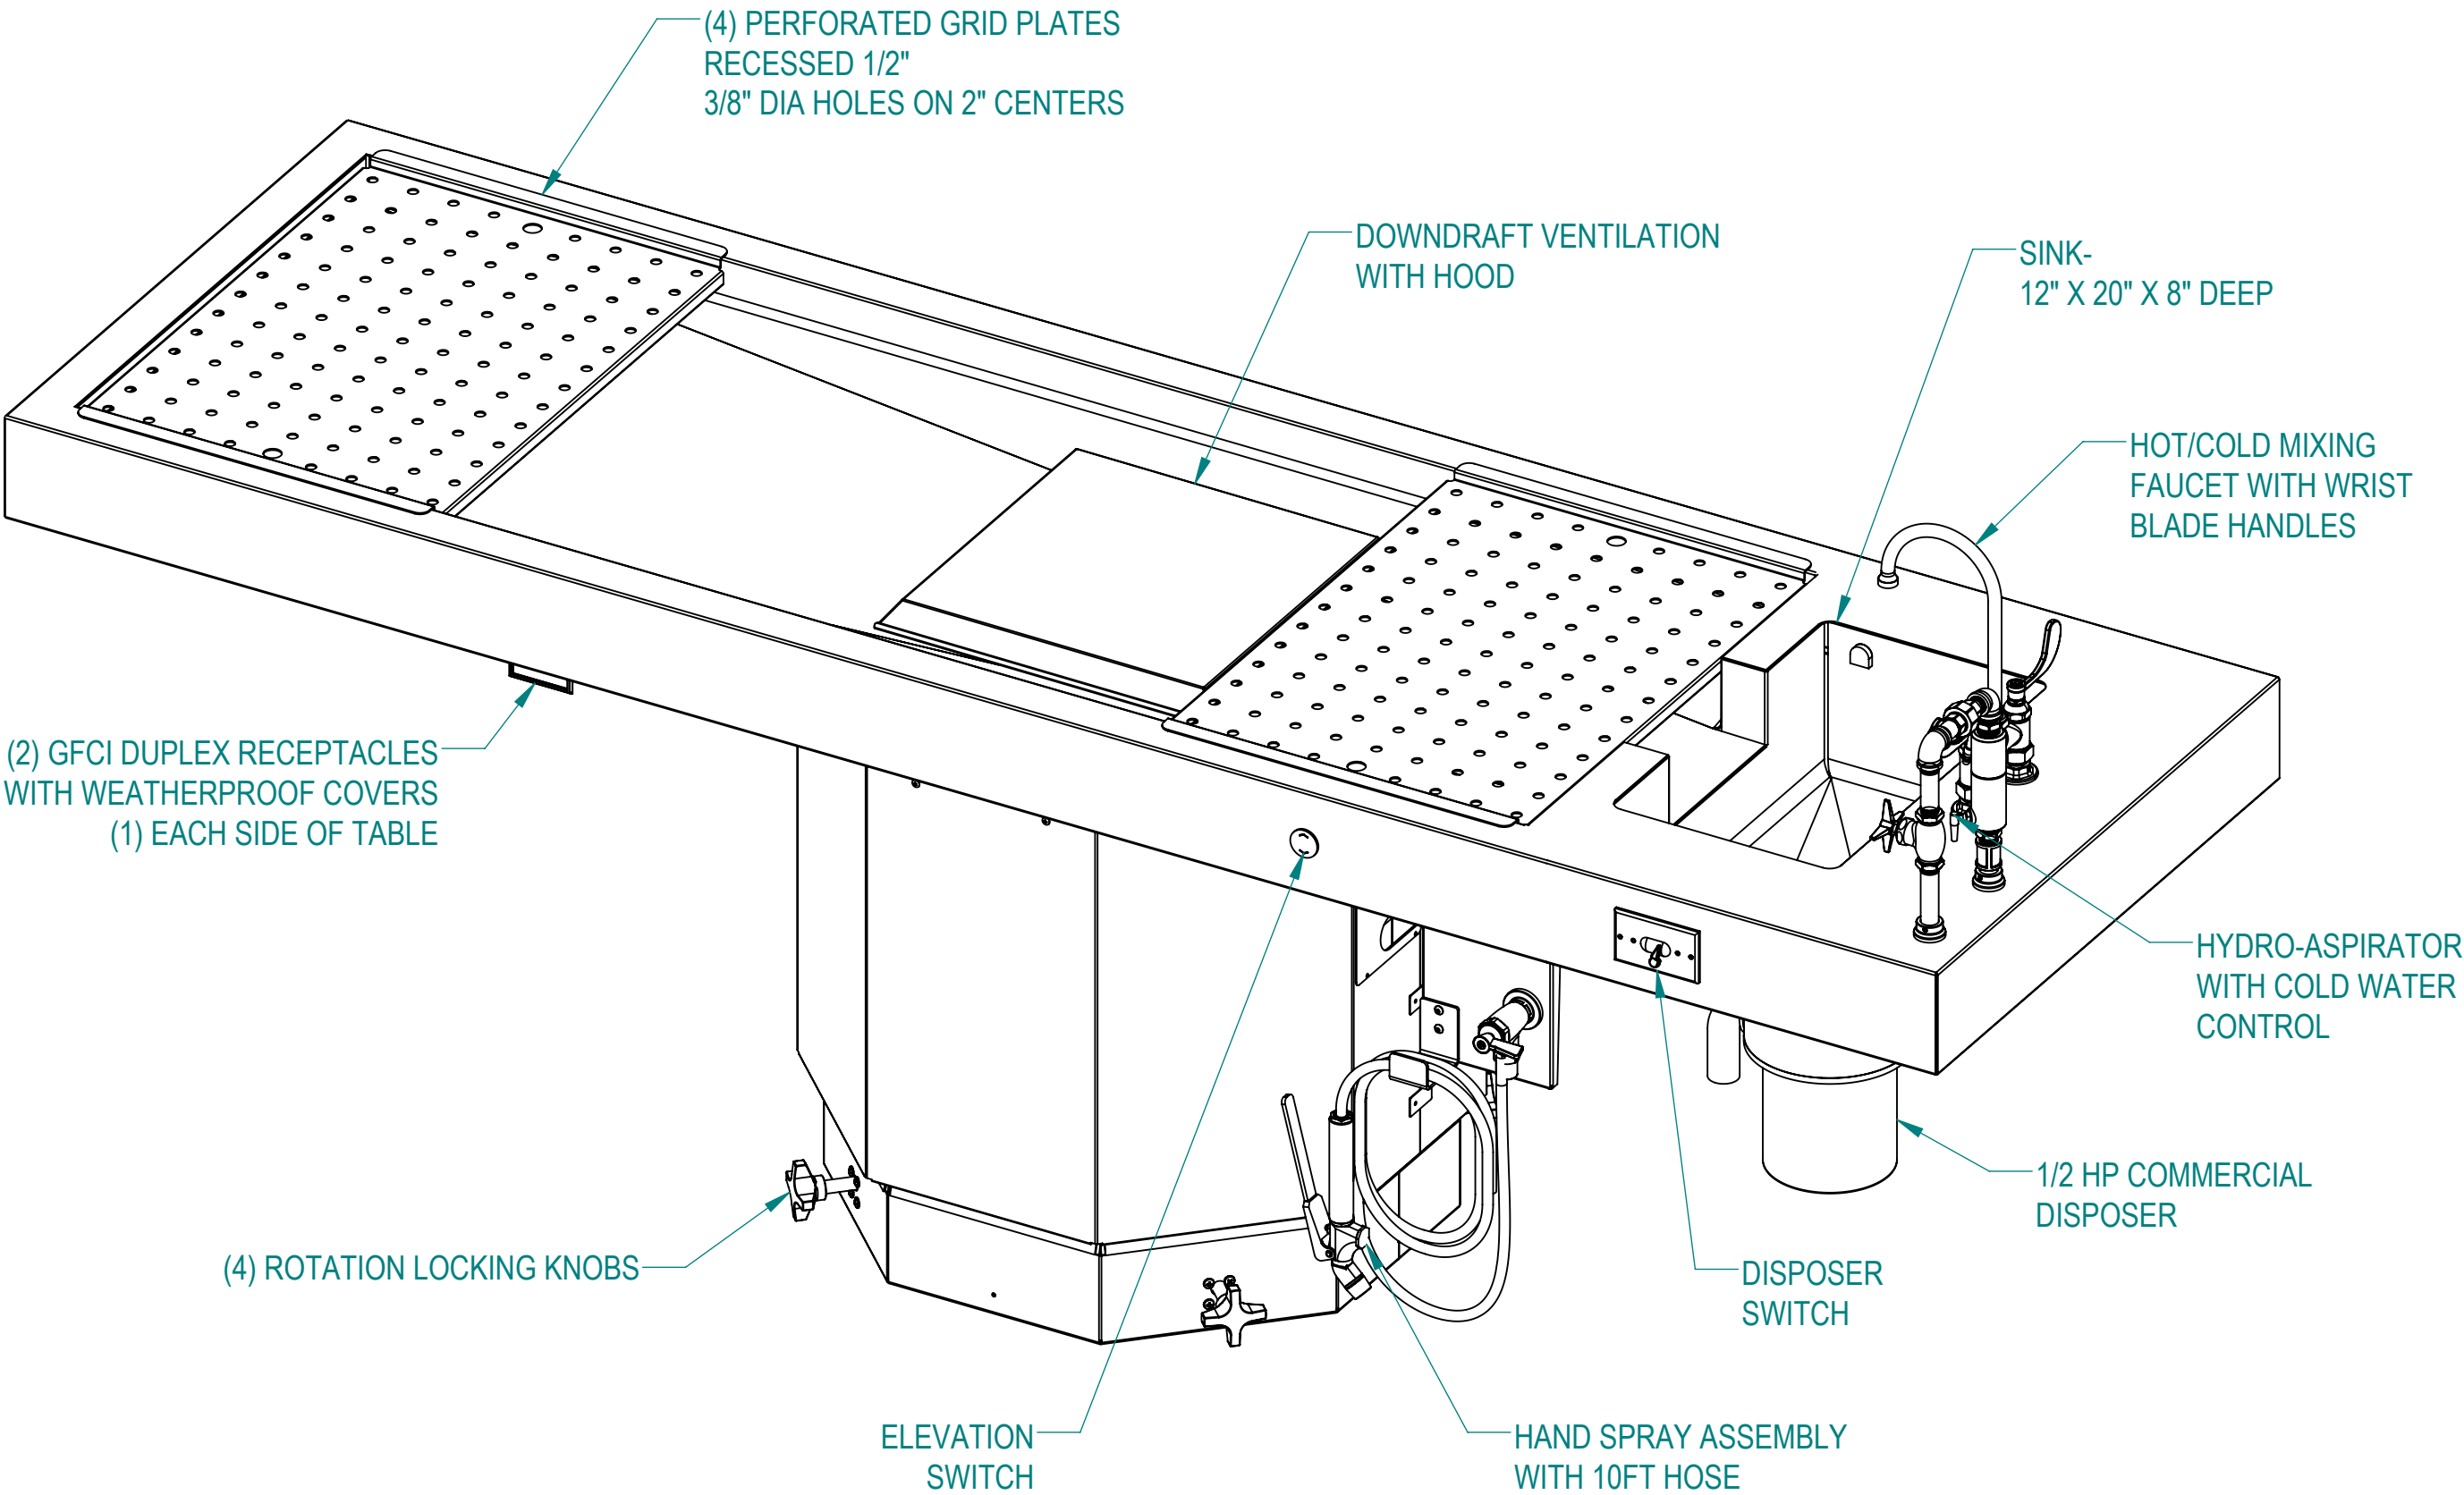

CUSTOMER		APPROVAL		PROPRIETARY THIS DOCUMENT AND THE DATE DISCLOSED HEREIN AND HEREWITH IS NOT TO BE REPRODUCED, USED, OR OTHERWISE DISCLOSED IN WHOLE OR IN PART TO ANYONE WITHOUT WRITTEN AUTHORIZATION FROM MOPEC GROUP.			MOPEC GROUP		Mopec ELEVATING PATHOLOGY MORTECH A Division of Mopec Group		411 North Aerojet Avenue Azusa, CA 91702 tel: (800) 410-0100 (626) 334-1471 fax: (626) 334-1704 www.mopecgroup.com						
PROJECT							DO NOT SCALE DRAWING		APPROVALS		DATE		TITLE MODEL 1036-48-MG (CE310) PEDESTAL AUTOPSY TABLE, ELEVATING & ROTATING				
		SIGNATURE		DATE		MATERIAL 304 STAINLESS STEEL		DRAWN BY ELISEO S.		03/27/25		SIZE C		DWG NO. 1036-48-MG		REV. A	
						FINISH #4		APPROVED BY				SCALE 1:8		NEXT ASSY.		SHEET 2 OF 3	

UTILITY REQUIREMENTS

1. INLET PLUMBING
- 1A. (1) COLD WATER SUPPLY, 1/2" OD COPPER STUBBED OUT 6"
- 1B. (1) HOT WATER SUPPLY, 1/2" OD COPPER STUBBED OUT 6"
- SUPPLY SHUT-OFF VALVES AT EACH WATER SUPPLY
2. (1) 2" DRAIN. (SEE DRAIN DETAIL)
3. A 4" X 4" AREA FOR ELECTRICAL INPUT TO INCLUDE THE FOLLOWING:
- (1) 115V/60Hz/1PH/20A CIRCUIT FOR STATION
- (1) 115V/60Hz/1PH/20A CIRCUIT FOR DISPOSAL
4. PROVIDE 60-65 PSI WATER PRESSURE AND 4 GALLONS PER MINUTE OF FLOW FOR PROPER OPERATION OF HYDRO-ASPIRATOR
5. ELECTRICIAN TO PROVIDE LIQUID TIGHT JUNCTION BOX AND CONDUIT PER LOCAL CODES.
6. FLUSH LINES CLEAR BEFORE CONNECTING TO STATION.
7. EXHAUST RECOMMENDATION:
- 275-400 CFM. EXISTING CONDITIONS MAY WARRANT AN INCREASE OR DECREASE, CONTACT YOUR ENGINEERING DEPT.

